



UHPC Software User Manual:

Version 2.8

© Avrion Battery Labs., 2026



Contents

1. UHPC System Introduction.....	4
2. Definitions.....	5
3. System Safety Overview	7
3.1 Standard Monitoring	7
3.2 Safety Limits.....	7
4. Software Download and Installation	9
4.1 Software Download.....	9
4.2 Software Installation	9
4.2.1 Software Installation	9
4.2.2 First Time PC IP Address Setup	9
5. UHPC Control Software User Manual	13
5.1 Main Control Software Operation	13
5.1.1 Menu Options	14
5.1.2 Channel Control Grid.....	17
5.1.3 System Log Panel	20
5.1.4 Selected Channels & Batch Control Panel.....	21
5.1.5 Protocol Step List Panel	21
5.1.6 Batch Control	25
5.1.7 Startup Configuration	28
5.1.8 Diagnostics.....	29
5.1.9 Column Configuration	31
5.1.10 Safety Limits.....	32
5.1.11 Restart from Previous Snapshot Data.....	32
5.1.12 Temperature Linking.....	35
5.1.13 Voltage Linking.....	36
5.1.14 Snapshots with Voltage and Temperature Links	37
6. UHPC Protocol Software Designer Manual.....	38
6.1 Main Protocol Software Operation.....	38
6.1.1 Control Options	39
6.1.2 Control Conditions.....	43
6.1.3 Step Safety Limits	45
6.1.4 Step Manipulation	46
6.1.5 Menu Options.....	48



6.1.6 Global Limits.....	51
6.1.7 Default Configurations.....	51
7. UHPC Plot Data Analysis Manual.....	53
7.1 UHPC Plot Software Operation	53
7.2 Data File Panel and Graph Settings Bar.....	54
7.2.1 Data File Panel	54
7.2.2 Graph Settings Bar.....	57
7.3 Graph Panels	59
7.4 Data File Formatting	61
7.5 Configuration Files	62
Appendix A – Temperature Control	63
Connecting a Thermal Chamber to UHPC Control.....	63
Setting Temperature with UHPC Protocol	66
Temperature Control with Multiple Channels.....	67
Temperature Linking	67
Appendix B – Gamry EIS Integration	69
First Time Gamry Hardware Setup.....	69
Connecting Gamry Hardware to PC and Updating Gamry Firmware.....	74
Connecting an EIS Device to UHPC Control	75
IMX8 Multiplexer	77
Viewing EIS Channel Information.....	78
Creating EIS test with UHPC Protocol.....	79
Running EIS Test with UHPC Control.....	83
Safety Warnings	84
Viewing EIS Data	84
Appendix C – API Remote UHPC Control Interface	85
API Configuration	86
UHPC Control API Message Format.....	87
Get Channel Status.....	90
Set Channel Info.....	91
Start Channel.....	92
Stop Channel	92
Suspend Channel.....	92
Resume Channel	93
Clear Channel Info	93



Sample Message Responses	93
Contact Us.....	95



1. UHPC System Introduction

Avrion's Ultra High Precision Coulometry (UHPC) battery testing systems offer industry leading accuracy and precision for battery test electronics. Each channel can operate in constant current or constant voltage charge and discharge modes across the full 0 – 5 V load window. Systems typically come with integrated thermal chambers to ensure the temperature stability of the cell to minimize noise, and eliminate temperature variations, in collected data. In addition to the thermal chamber temperature monitoring, each channel connected to a cell holder and RTD constantly monitors local cell temperature and reports it to the UHPC Control software. When used under appropriate conditions, each channel can measure coulombic efficiency to better than 20 ppm precision and better than 50 ppm accuracy.

The software allows users to easily build test protocols to start experiments and monitor the status of each channel. Data analysis software outputs data in various formats for ease of analysis and understanding of cell performance.

The system is to be used as delivered, not modified or controlled by external software. The unit is used for testing electrochemical cells within the known limits between 0-5 volts in different operation modes (constant current charge/discharge, constant voltage charge/discharge or open circuit storage). This includes devices like rechargeable batteries (all chemistries) and supercapacitors.

2. Definitions

Filename abbreviation	Symbol	Description	Units
-	V_L	Lower voltage limit for standard cell cycling (Fig 1)	V
-	V_U	Upper voltage limit for standard cell cycling (Fig 1)	V
Q_c	Q_C	Charge capacity for the cell (charged from V_L to V_U) (Fig 1)	Ah
Q_d	Q_D	Discharge capacity for the cell (discharged from V_U to V_L) (abs. value) (Fig 1)	Ah
CE	CE	Coulombic efficiency: $CE = \frac{Q_D(n)}{Q_C(n)}$	unitless
CIE	CIE	Coulombic inefficiency: $CIE = 1 - CE$	unitless
CIE_{hr}	CIE/hr	Coulombic inefficiency per hour: $CIE/hr = \frac{(1-CE)}{\text{cycle time}}$	hour ⁻¹
$CendPt$	EP_C	Charge endpoint capacity: $EP_C(n) = EP_D(n-1) + Q_C(n)$	Ah
$DendPt$	EP_D	Discharge endpoint capacity: $EP_D(n) = EP_C(n) + Q_D(n)$	Ah
$SlipC$	Δ_C	Charge slippage: $\Delta_C(n) = EP_C(n) - EP_C(n-1)$ (Fig 2)	Ah
$SlipD$	Δ_D	Discharge slippage: $\Delta_D(n) = EP_D(n) - EP_D(n-1)$	Ah
$SlipCpercent$	$\Delta_C\%$	Charge slippage percent: $\Delta_C\% = \Delta_C(n)/Q_C(n) * 100$	%
$SlipDpercent$	$\Delta_D\%$	Discharge slippage percent: $\Delta_D\% = \Delta_D(n)/Q_D(n) * 100$	%
$Fade$	$Fade$	Capacity fade: $Fade = \Delta_C - \Delta_D$	Ah
$ZeroedCendPt$	EP_C^0	Zeroed charge endpoint capacity: $EP_C^0 = EP_C(n) - EP_C(n = ref)$	Ah
$ZeroedDendPt$	EP_D^0	Zeroed discharge endpoint capacity: $EP_D^0 = EP_D(n) - EP_D(n = ref)$	Ah
$Qcpercent$	$Q_C\%$	Capacity charge percent: $Q_C\% = Q_C(n)/Q_C(n = ref) * 100$	%
$Qdpercent$	$Q_D\%$	Capacity discharge percent: $Q_D\% = Q_D(n)/Q_D(n = ref) * 100$	%
$CendPtPercent$	$EP_C\%$	Charge endpoint capacity percent: $EP_C\% = EP_C(n)/EP_C(n = ref) * 100$	%
$DendPtPercent$	$EP_D\%$	Discharge endpoint capacity percent: $EP_D\% = EP_D(n)/EP_D(n = ref) * 100$	%
$AvgVc$	V_{avgC}	Average charge voltage: $V_{avgC} = \int_0^{Q_C} V dQ$	V
$AvgVd$	V_{avgD}	Average discharge voltage: $V_{avgD} = \int_0^{Q_D} V dQ$	V
$DeltaV$	ΔV	$\Delta V = V_{avgC} - V_{avgD}$	V
$dVdQ$	dV/dQ	Differential capacity $\frac{dV}{dQ}(n) = \frac{V(n)-V(n-1)}{Q(n)-Q(n-1)}$	VAh ⁻¹
$dQdV$	dQ/dV	Differential voltage $\frac{dQ}{dV}(n) = \frac{Q(n)-Q(n-1)}{V(n)-V(n-1)}$	AhV ⁻¹
$Vdrop$	ΔV_{st}	Voltage drop during storage – the change in voltage from when a cell starts open circuit storage to the time the cell starts charging or discharging again	V

E_C	E_C	Charge energy: $E_C = Q_C * V_{avgC}$	Wh
E_D	E_D	Discharge energy: $E_D = Q_D * V_{avgD}$	Wh
EE	EE	Energy efficiency: $EE = E_D(n) / E_C(n)$	unitless
$E_{Cpercent}$	$E_C\%$	Energy charge percent: $E_C\% = E_C(n) / E_C(n = ref) * 100$	%
$E_{Dpercent}$	$E_D\%$	Energy discharge percent: $E_D\% = E_D(n) / E_D(n = ref) * 100$	%

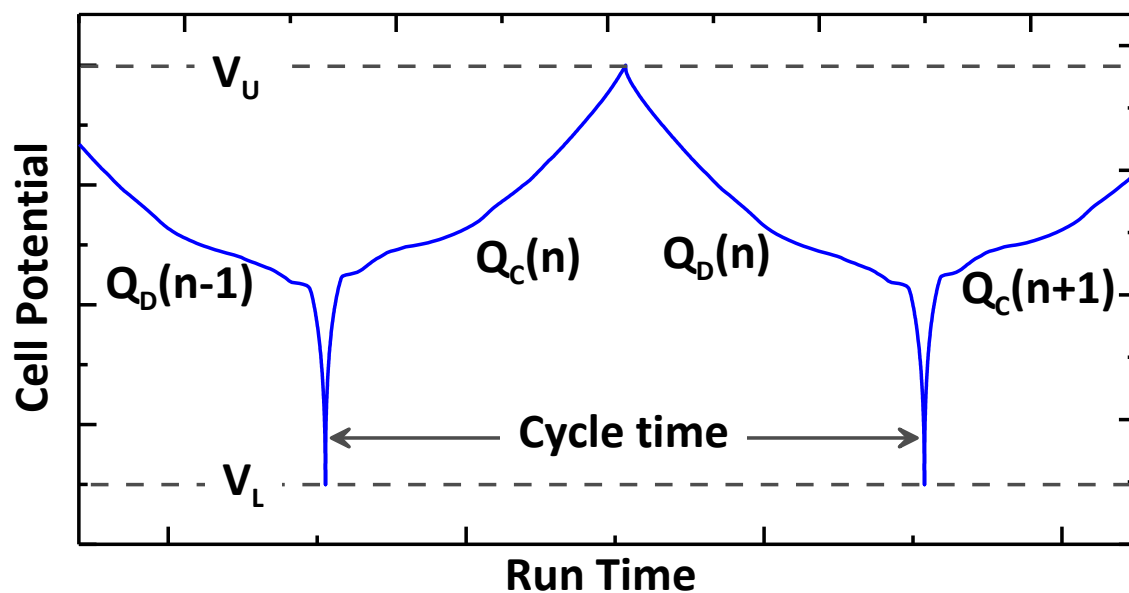


Figure: An example of a voltage versus run time plot displaying the parameters lower voltage limit (V_L), upper voltage limit (V_U), charge capacity (Q_C), discharge capacity (Q_D) and cycle time.

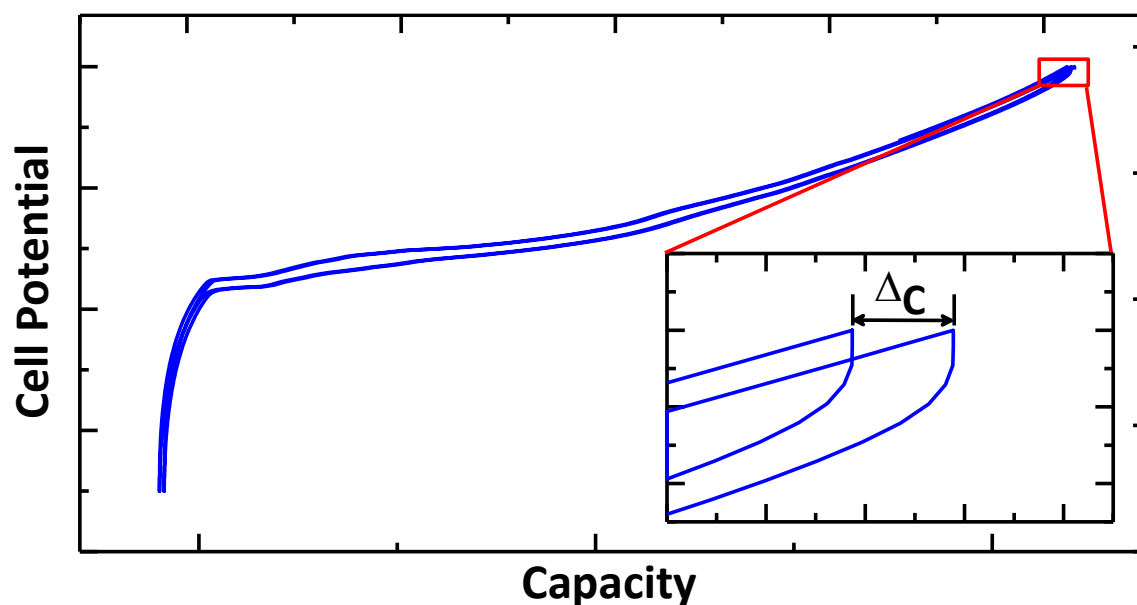


Figure: An example voltage versus capacity curve with an inset showing the charge slippage (ΔC).



3. System Safety Overview

UHPC systems comprise of various software applications, channel modules, thermal chambers, control module and PC. Safety is designed into the system and outlined below.

3.1 Standard Monitoring

Standard monitoring continuously runs on all systems, to ensure that unexpected conditions do not persist. Standard monitoring tracks:

- Occurrence of bad values
- Current set point stability
- Voltage set point stability
- Inactive channels
- System connections
 - Between PC and control module
 - Between control module and channel module
 - Between each channel and control module

Should any anomalies be recognized by standard monitoring, the system will isolate offending channels, thereby breaking the physical current connection. Further, the current set point is reduced to near zero as a secondary precaution.

3.2 Safety Limits

Safety Limits are the UHPC Control's system emergency test safety measures. When breached, the system will begin test shutdown. This specific behavior can be modified in Startup Configuration to either stop all tests, suspend the impacted test, or by default: Stop the impacted test. Safety Limits can have three levels. In order of hierarchy, they are:

1. **System Limits** – System Limits are set before shipment and cannot be changed. These can only be viewed in UHPC Control. The system limits are the top hierarchy, and all types of limits must be within the range of system limits.
2. **Global Limits** – Global limits are shared between UHPC Protocol and UHPC Control, they require an admin password to edit. The Global Limits must be within the System Limits. These limits are enforced on all protocols loaded/running in UHPC Control. When Global limits are breached, the test will generally stop, although it can be configured to suspend the channels instead.
3. **Step Limits** – Step Limits are fully customizable by the user, without requiring any admin password. They can be set in UHPC Protocol. Step limits should be within Global Limits and are identical to global limits by default. You can set custom limits, so that your tests stop or suspend if a certain threshold was breached during testing. The intent of Step Limits is for the user to be able to configure more constrained step specific (or test specific) limits without impacting every test executing on UHPC Control.



For the Global and Step Safety Limits, an Operating Limit can be set for:

Channel Current (A), Cell Voltage (V), and Cell Temperature (C)

Should the Operating Limit be met or exceeded, then the non-compliant channel will be isolated and have Channel Current set-point set to near zero. If the user has configured the system to shut down all channels on reached limit, then all channels will be isolated and have Channel Current set-point set to zero. Any changes to the thresholds must be made with appropriate user permission.

Limits are set to the following values, before shipment:

	System Limits		Global Limits		Step limits	
	Min	Max	Min	Max	Min	Max
Channel Current (A) – 2 Amp	0	2.2	0	2.05	0	2.05
Channel Current (A) – 10 Amp	0	10.2	0	10.05	0	10.05
Channel Current (A) – 20 Amp	0	20.2	0	20.05	0	20.05
Cell Voltage (V)	0	5.2	0	5	0	5
Cell Temperature (°C)	-150	500	-50	80	-50	80

For further information and support, please [contact us](#).



4. Software Download and Installation

4.1 Software Download

Three software programs are supplied with a system. Software and user manual can be found in [Avrion Customer Area](#). Please [contact us](#) if further information is needed.

UHPC Control: This program communicates with the connected channel modules via the connected master controllers. Monitoring the cells voltage, current, and temperature, while also executing the user defined protocol files, and controlling charge/discharge profiles of the channel modules.

UHPC Protocol: This program is used to generate the test sequence protocol files that dictate how a charger channel will operate for a given cell. It allows the user to configure currents, voltage limits, data collection intervals etc.

UHPC Plot: This program allows the user to analyze data files generated by the UHPC Control software. It provides both a graphical interface for viewing of data and a data export section that allows the user to export simple text files for subsequent graphing and further analysis.

4.2 Software Installation

4.2.1 Software Installation

If updating from any version's earlier than 2.5.0, the software will need to be manually uninstalled from Windows "Add Remove Programs" after updating the software. Otherwise, for all later versions the installer will automatically replace the current installation, so ensure that the UHPC Control software is not running during installation.


1. Run the .msi file in the .zip folder provided by Avrion containing the UHPC software.
2. Install to the default directory.
3. Launch the application.
4. Once installed, read this UHPC manual (In the software toolbar: Help -> Help Manual) for up-to-date information on how to operate the software.
5. All previous settings and configurations should remain unless otherwise stated in the release notes.

4.2.2 First Time PC IP Address Setup



This will have been completed for Avrion supplied UHPC Desktop PC's, but in the case of replacement PC's or third-party PC's the following steps will need to be completed to set up the network configuration to communicate with the UHPC hardware.

The two default IPs are "172.29.9.1" and older systems may be "192.168.1.1".

A quick explanation can be found below though in Figure 1 and Figure 2.
In the Windows search bar type and left click "View network connections".



- Right click the unidentified network (master controller). Click “Properties.”

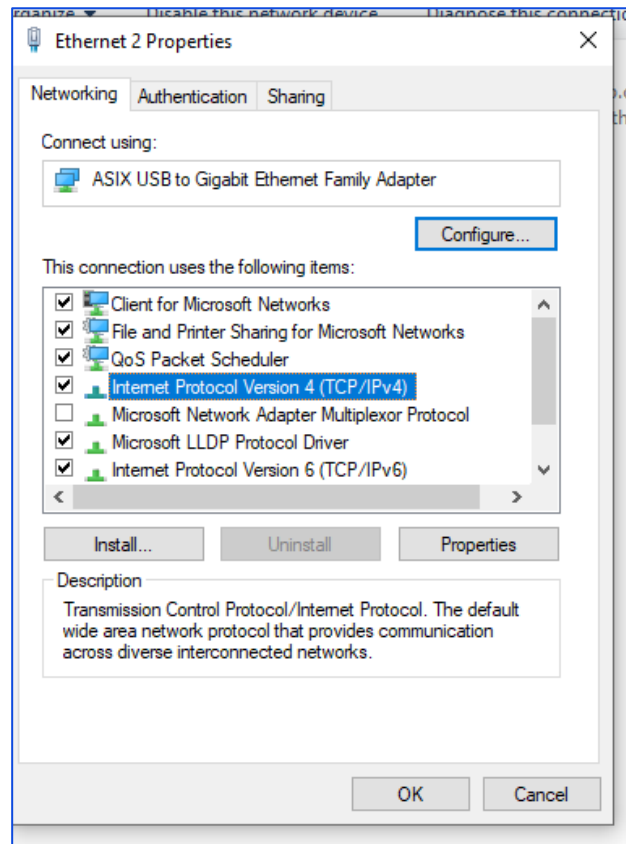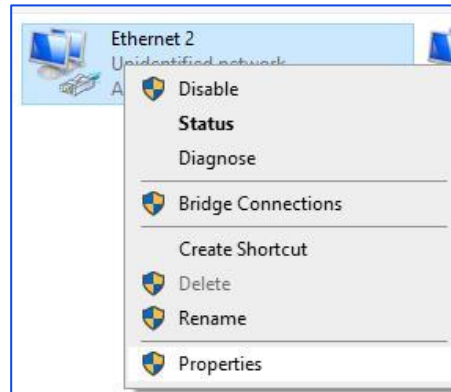

- In properties, click the “IPv4”.

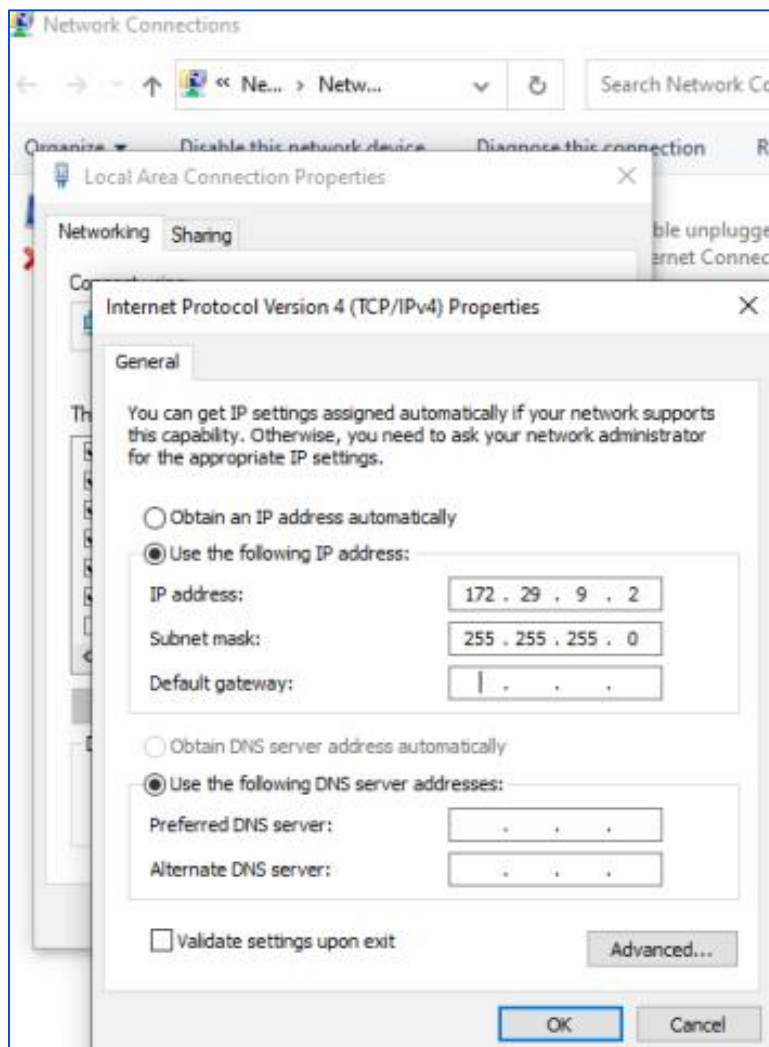


Figure 1: Navigating to PC Network Configuration

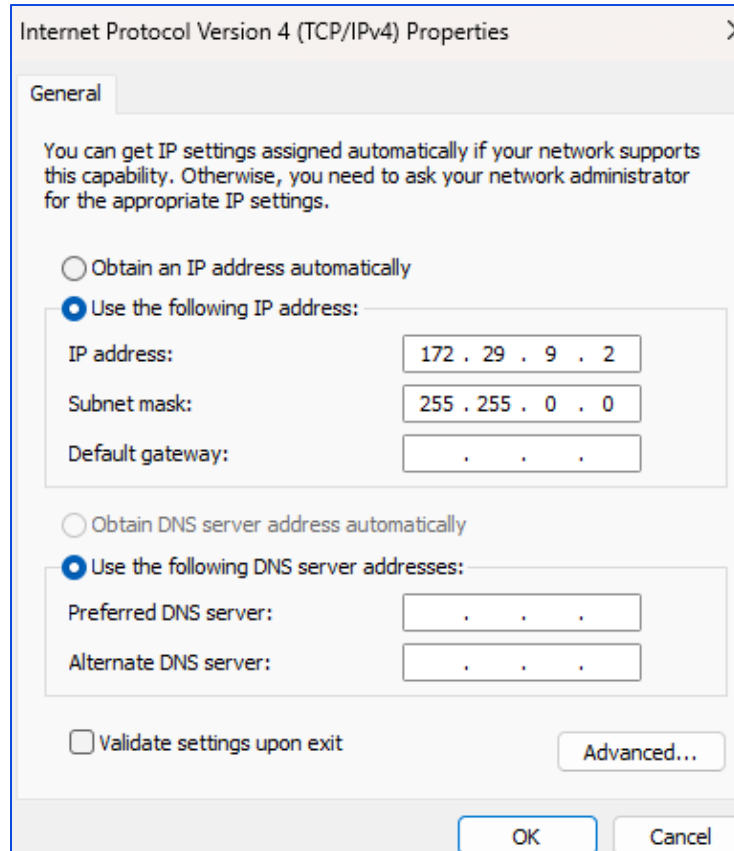


Figure 2: PC Network Configuration

- Once the user has navigated to the IPV4 configuration page, the IP Address should be filled out with one of the two default IP's given above, **but with the following exception:** The final digit should be incremented by at least 1. This is to establish a standalone network for connection.
- After setting the IPV4 configuration, try running “Troubleshoot Network” from UHPC. If it fails, adjust the IPV4 to the other unique IP given above, increment the final digit by 1, and try again.



5. UHPC Control Software User Manual

5.1 Main Control Software Operation

After the channel control module has fully powered up and all channel modules are operational (wait 30 seconds after powering ethernet module before turning on channel modules), the UHPC Control software can be started. A shortcut can be found on the desktop.

The main screen will look like this, varying based on channel count and selected settings:

NOVONIX | UHPC Control

File Tools Settings Help

Channel Type Filter: Idle Running Loaded Suspended Completed Disabled Restart from previous channel snapshot 2A

Channel Control Panel

Channel	Append Data	Description	Barcode	Cell ID	Mass (g)	Cap. (pF)	Data File Name	Protocol File Name	Temp	Run Time	Step Time	Current	Potential	Step Capacity	Cycle Num	Active Step
1	Start	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	21.214°C	---	---	0	1.74056662 V	---	---	---
2	Start	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	20.440°C	---	---	0	3.33409493 V	---	---	---
3	Start	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	20.784°C	---	---	0	2.91446383 V	---	---	---
4	Start	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	20.438°C	---	---	0	3.62144819 V	---	---	---
5	Start	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	20.598°C	---	---	0	2.17519177 V	---	---	---
6	Start	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	20.457°C	---	---	0	1.93129434 V	---	---	---
7	Start	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	20.473°C	---	---	0	1.65388482 V	---	---	---
8	Start	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	---	---	---	0	1.2733529 mV	---	---	---
9	Disabled	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	---	---	---	-9999	Out of Range	---	---	---
10	Disabled	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	---	---	---	-9999	Out of Range	---	---	---
11	Disabled	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	---	---	---	-9999	Out of Range	---	---	---
12	Disabled	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	---	---	---	-9999	Out of Range	---	---	---
13	Disabled	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	---	---	---	-9999	Out of Range	---	---	---
14	Disabled	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	---	---	---	-9999	Out of Range	---	---	---
15	Disabled	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	---	---	---	-9999	Out of Range	---	---	---
16	Disabled	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	---	---	---	-9999	Out of Range	---	---	---
17	Disabled	Enter description here...			1.000	1.000	Click to select data file...	Click to select protocol file...	---	---	---	-9999	Out of Range	---	---	---

Protocol Step List (No Channel Currently Selected)

Protocol Step List for Channel: Expanded

Communication Log View Communication Log Clear

System Log Panel

Error Log View Error Logs Clear

Selected Channels

Batch Control Stop Suspend

Selected Channel Panel & Batch Control

Figure 3: Main screen layout panels

5.1.1 Menu Options

File Menu

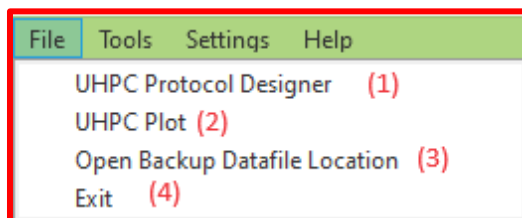


Figure 4: File drop-down list menu

UHPC Protocol Designer (1):

This launches the UHPC Protocol Designer program, which is used to generate test protocols that documents the series of control steps to be run on channel that are assigned that protocol file (*.pro1, *.pro2).

More information on UHPC Protocol can be found in the [UHPC Protocol Software Designer Manual](#) portion of this document.

UHPC Plot (2):

This launches the UHPC Plot program that is used to analyse the data files collected and generate summary data files for subsequent graphing with external programs such as Open Office®, Microsoft Excel®, Golden Software Grapher®, etc. This program allows the user to view graphical representations of the data collected both when cells are running and after testing.

More information on UHPC Plot can be found in the [UHPC Plot Data Analysis Manual](#) portion of this document.

Open Backup Datafile Location (3):

This opens the datafile folder found in C:/Avrion/UHPC Backup containing the backups to channels recently ran on the current network configuration. These files are held in this folder typically forever, or until a test with a duplicate file name is ran.

Exit (4):

This will prompt the user to confirm that they wish to shut down all channels and close the program.

Tools Menu




Figure 5: Tools drop-down list menu

Diagnostics (1):

Tool for troubleshooting network issues, flashing LED's on specific channels, and generating diagnostic reports for troubleshooting with UHPC customer support. In diagnostics, password restricted advanced diagnostic controls can also be found for communicating with the channel modules manually.

For customer support, please see the [contact us](#) section of this document.

Settings Menu

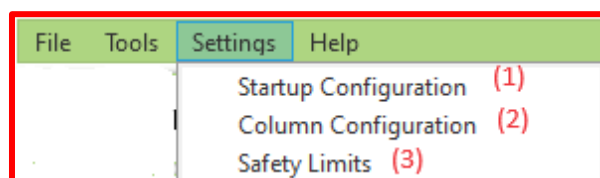


Figure 6: Settings drop-down list menu

Startup Configuration (1):

Configures settings that affect the program at start-up. This menu is described further in the [Startup Configuration](#) section.

Column Configuration (2):

Change column names and set whether they should be displayed or hidden. This menu is described further in the [Column Configuration](#) section.

Safety Limits (3):

Check and set safety limits used to monitor channels and alert if limits breached. This menu is described further in the [Safety Limits](#) section.

Help Menu




Figure 7: Help drop-down list menu.

Getting Started First Test (1):

Launches the Getting-Started-First-Test.pdf to help users set up and execute their first UHPC test.

System Manual (2):

Launches the System Manual for the UHPC Control Hardware.

Help Manual (3):

Launches the Help Manual for the UHPC Control program (this document).

Release Notes (4):

Launches the release notes .pdf for the current UHPC Control program containing all the changes iterated by version.

Factory Reset (5):

Resets almost all UHPC Control configuration data. System limits, Global Limits, Startup Configurations, Column Configurations are all removed and set to default values. Snapshots and backups are retained.

Check for Update (6):

Manually makes a check with the UHPC customer portal to check for updates. This is also done automatically once daily unless the user disables it in Startup Configuration. No information is shared with Avrion or downloaded automatically during this call.

Contact Us (7):

Provides the user a popup containing the Avrion customer support email address, this information can also be found at the bottom of this document in the “Contact Us” section.

About (8):

Provides information on the Avrion UHPC Control program version and third-party licensing.

5.1.2 Channel Control Grid

Note: A number of these settings are toggleable in the settings menus.

Channel Type Filter : Idle 4 Running 1 Loaded 3 **Suspended 1** Completed 1 Disabled 0

				Channel	Description	Barcode	Cell ID	Mass (g)
2 Amp	Suspended	Stop	Resume	04	Enter description here...			1.000

Figure 8: Channel type filters display, with suspended channels selected.

Channel Type Filter:

Selecting an option (e.g., Idle, Running, Loaded, etc.) will display only the channels that fit the selection. Multiple types can be selected at one time. Selected filter types will be highlighted green. If no channel type filters are selected, then all channels will be shown.



Figure 9: Status indicator, as well as start and suspend buttons.

Status:

The status of the channel (shown above as “Idle”) will display the state of the channel at that moment.

Start button:

This button is only active for a given channel when it is in the idle state and loaded (i.e. both the protocol file and data file have been selected). Clicking on the button will immediately start the channel. Its label will change to Stop. This button can then be clicked to stop the channel. You will be prompted to confirm that you wish to stop the channel.

Suspend button:

This button is only active for a given channel once it is running a protocol file. Clicking on the button will prompt you for whether you wish to suspend operation of the channel. Selecting less will turn off current to the cell. The button’s caption will change to Resume. Clicking the button when it says Resume will immediately resume operation of the channel.


Channel:

The channel number for the row, starting at 1.

Append Data:

When checked, the user may select a pre-existing datafile. Data will be written to the end of the selected datafile. When Append Data is clicked, if a datafile is loaded already, or if a data file is loaded after clicking append data, Cell Capacity, Cell Mass, and Protocol File*(V2.10.0 datafile and above) will be loaded automatically in the data grid for the channel. Additionally, run time, Cumulative Capacity, Cycle #, and Step # will also be pulled from the last line on the existing datafile and used when starting the test. No header new lines will be written.

This option can be configured in Settings -> System Configuration -> Features -> Append Data Settings.

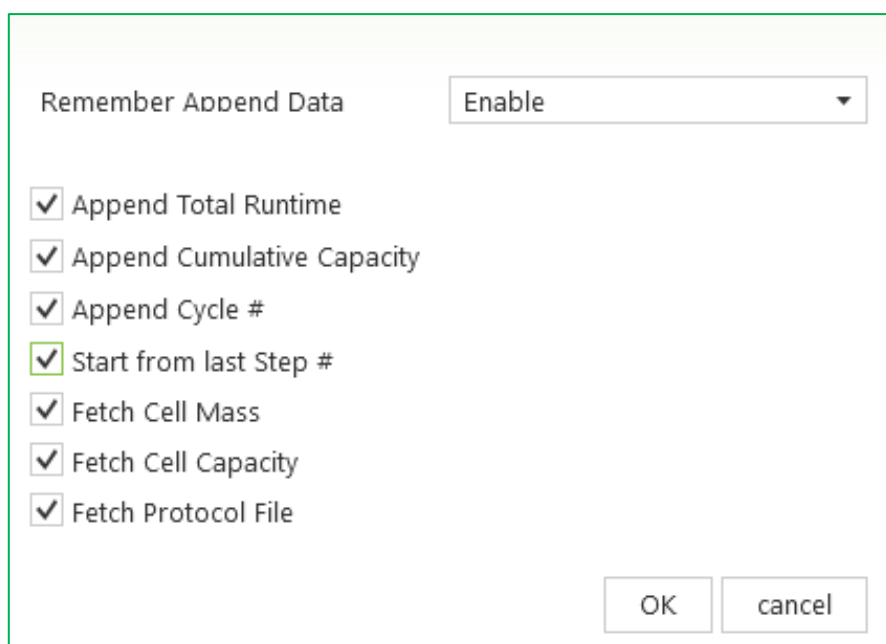

The image shows a dialog box titled "Append Data Settings". At the top, there is a label "Remember Append Data" followed by a dropdown menu currently set to "Enable". Below this, there is a list of seven checkboxes, all of which are checked:

- ☒ Append Total Runtime
- ☒ Append Cumulative Capacity
- ☒ Append Cycle #
- ☒ Start from last Step #
- ☒ Fetch Cell Mass
- ☒ Fetch Cell Capacity
- ☒ Fetch Protocol File

At the bottom right of the dialog box, there are two buttons: "OK" and "cancel".

Figure 10: Append Data Settings Window

Description column:

Allows the user to enter a text-based description to be written to the header of the data file. (The data file header also contains information such as channel number, date started, capacity, active mass, protocol file used, etc.)

Barcode:

Allows the user to enter a barcode description for the cell. The entered barcode will not impact anything.

Cell ID:

Allows the user to enter a cell ID description for the cell. The entered cell ID will not impact anything.

**Mass column:**

Allows the user to enter a cell active mass if using a protocol file that contains steps based on active mass (e.g., a current entered in A/g). If no mass is entered, this value will default to 1 g. If no specific currents are used in the test protocol, the entered mass will not impact anything.

Capacity column:

Allows the user to enter a cell capacity if using a protocol file that contains steps based on capacity (e.g., a current entered as a C-rate or a C/xx rate). If no capacity is entered, this value will default to 1 Ah. If no C-rates are used in the test protocol, the entered capacity will not impact anything.

Area column:

Allows the user to enter a cell area if using a protocol file that contains steps based on area (e.g., a current entered in A/cm²). If no area is entered, this value will default to 1 cm². If no specific currents are used in the test protocol, the entered mass will not impact anything.

Data file column:

Allows the user to select the data file to be used for a cell that they wish to run. Clicking on the label will bring up an explorer window pointing to the last directory where data was saved. Data is stored in a simple comma separated ASCII text format (*.csv file type). This file type will typically open by default with Microsoft Excel®, if installed.

Protocol file column:

Allows the user to select the test protocol file (created in the protocol designer - see the Protocol Step List Panel section and/or UHPC Protocol help document) to be used to run a file.

Channel status columns:

The Run time, Step time, Current, Potential, Step Capacity, Cumulative Capacity, and Cycle # columns provide information on the current state of the channel. The Active Step Display column shows a description of the protocol step currently running. Clicking on the label for a channel in this column will bring up a list of the steps to be run on that channel.

Chamber Name:

The Chamber Name is used to differentiate Avrion IP-enabled thermal chambers assigned to channels.

Chamber Temperature:

The Chamber Temperature displays the temperature for any channel with a connected IP-Enabled thermal chamber. If no configuration exists for that channel or the chamber is not connected, "---" will be displayed.



Linked EIS Device:

The Linked EIS Device column will display the associated EIS Channel # and the EIS Model # for any channel that has an EIS device assigned. To assign or unassign an EIS device, right click the channel and select “Assign EIS Device”.

5.1.3 System Log Panel

This panel provides a log of system events (starting and stopping channels, etc.).

Error Log	View Error Logs	Clear
228 2023-12-22 13:48:24 System Temporary controller connection issue		
229 2023-12-22 13:48:29 System Temporary controller connection issue		
230 2023-12-22 13:48:34 System Temporary controller connection issue		
231 2023-12-22 13:48:39 System Temporary controller connection issue		

Figure 11: Error log displaying controller connection issues.

Communication Log	View Comm Logs	Clear
227 December 22, 2023 - 01:47:53 PM System Opening communication link		
228 December 22, 2023 - 01:47:58 PM System Opening communication link		
229 December 22, 2023 - 01:48:03 PM System Opening communication link		
230 December 22, 2023 - 01:48:08 PM System Opening communication link		

Figure 12: Communication log showing communication links being opened.

View Error Logs:

Opens the default Windows Explorer folder for the error logs. (C:\Avrion\UHPC Log Files\ErrorLogs)

View Comm Logs:

Opens the default Windows Explorer folder for the communication logs. (C:\Avrion\UHPC Log Files\{System Name})

Clear:

Clears the logs displayed on the screen. To permanently delete logs, use the View Error Logs/View Comm logs buttons and delete files using windows file deletion.

5.1.4 Selected Channels & Batch Control Panel

Displays all channels currently selected (selected panels will be highlighted on the control panel).

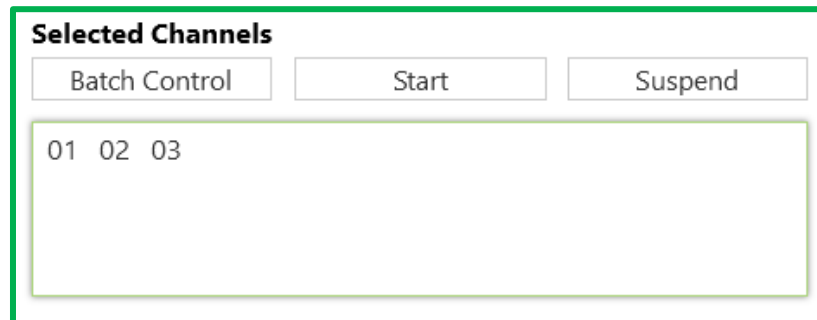


Figure 13: The selected channels panel, with three channels (01, 02 and 03) selected.

Batch Control:

Will bring up a window to assign values to all the channels in the “Selected Channel” list shown above. (See the Batch Control Panel section for more details).

Start:

Used as a quick batch command to start all channels selected. If all channels currently selected are running the button will switch to “Stop.” If there is a mix between running and idle channels, this button will be disabled.

Suspend:

Used as a quick batch command to suspend all channels selected. If all channels currently selected are suspended the button will switch to “Stop.” If all channels selected are not either suspended or running, this button will be disabled.

5.1.5 Protocol Step List Panel

The protocol step list panel displays the protocol file of the currently selected channel. If multiple channels are selected, the first channel that was selected will be displayed. The user has right click options on each step in the protocol step list. Each protocol step action can only be applied to one step per channel at a time.

Protocol Step List:

This view of the control software represents the condensed view that shows looping steps.

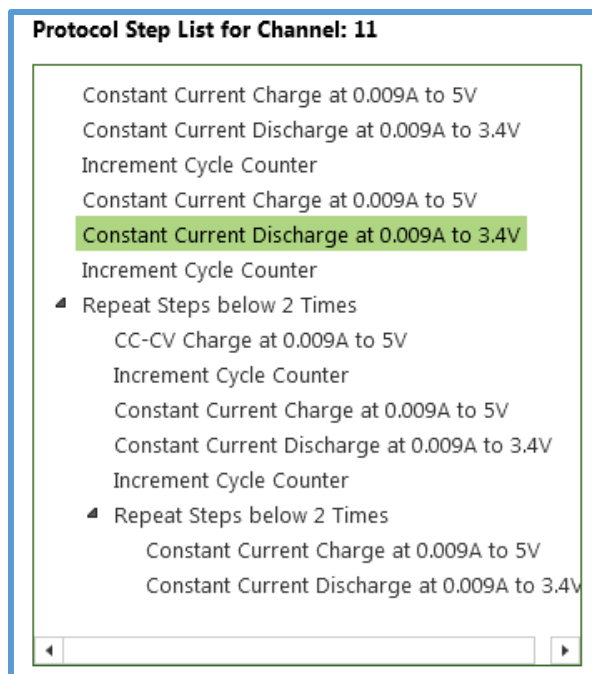


Figure 14: Condensed protocol step list view.

Protocol Step List (Expanded):

This view of the control software represents all the steps expanded out in the sequential order in which they will be executed.

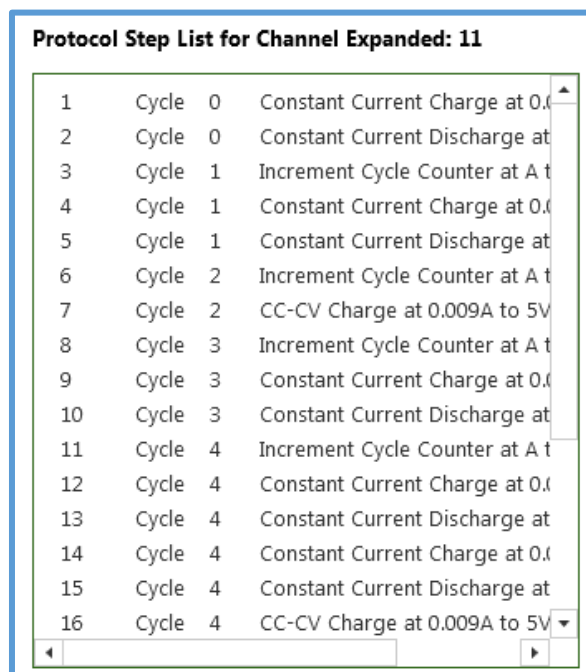


Figure 15: Expanded protocol step list view.

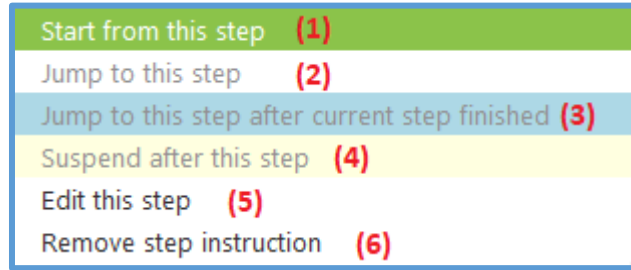


Figure 16: The protocol step list right-click menu.

Start from this step (1):

If the channel is in the Idle state, this option allows the user to run the channel from the step selected.

Jump to this step (2):

This command will cause the channel to immediately go to the step selected, ending the current running step. If the channel is suspended, using this command will resume the channel as well.

Jump to this step after current step finished (3):

If the channel is running, using this command will cause the channel to navigate to the step selected after the current step is finished. This command causes the selected step to be highlighted in blue in the expanded protocol step list.


Suspend after this step (4):

After selecting this option on a step, when that step finishes the channel will be suspended until manually resumed. This command causes the selected step to be highlighted in yellow in the expanded protocol step list.

Edit this Step (5):

After selecting this open, an edit step conditions dialog box will appear, as shown in Figure 17. Currently only Current, Units, and Voltage target may be edited.

Warning: This change has not yet persisted across snapshots. When resuming from snapshots, be sure that any changes that are still required for current or future steps are adjusted accordingly.

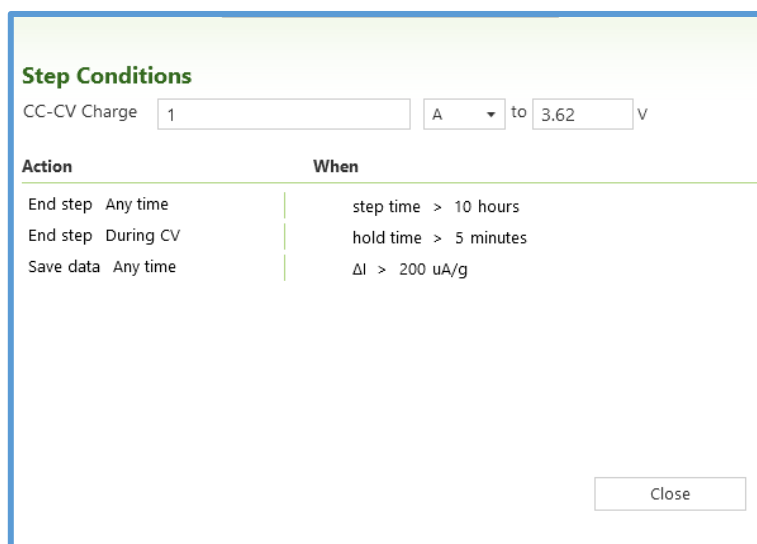

Step Conditions

CC-CV Charge A to V

Action	When
End step Any time	step time > 10 hours
End step During CV	hold time > 5 minutes
Save data Any time	$\Delta I > 200 \text{ uA/g}$


Close

Figure 17: Edit Step Conditions Dialog Box

Remove Step Instruction (5):

Available only in 'expanded' mode of protocol list, after selecting this option on a step, this command causes the selected step to be removed from the protocol list. Only future steps may be removed.

Warning: This change has not yet persisted across snapshot saves; If the test is resumed from snapshot after the test has passed a removed step, unintended behavior can occur. In these cases, be sure to jump to the correct step after restarting from snapshot.

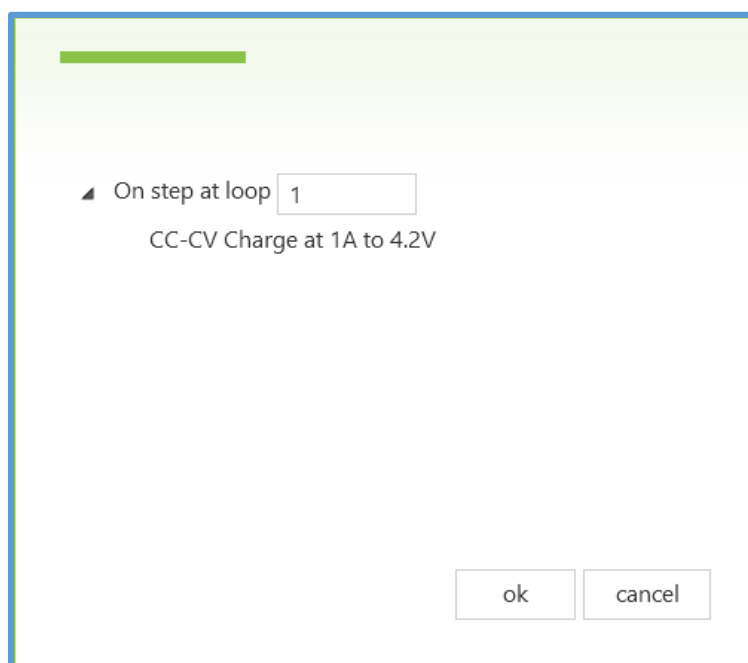

On step at loop

CC-CV Charge at 1A to 4.2V

ok cancel


Figure 18: Loop menu displayed when making an action to a step in condensed view.

Choosing position in repeating steps:

When choosing one of the right-click options outlined above in compact protocol step list view, a window will pop up prompting the user to specify the loop number to execute the action within.

5.1.6 Batch Control

This feature assigns values to all the channels in the “Selected Channel” list, as described above in the Selected Channels Panel section.

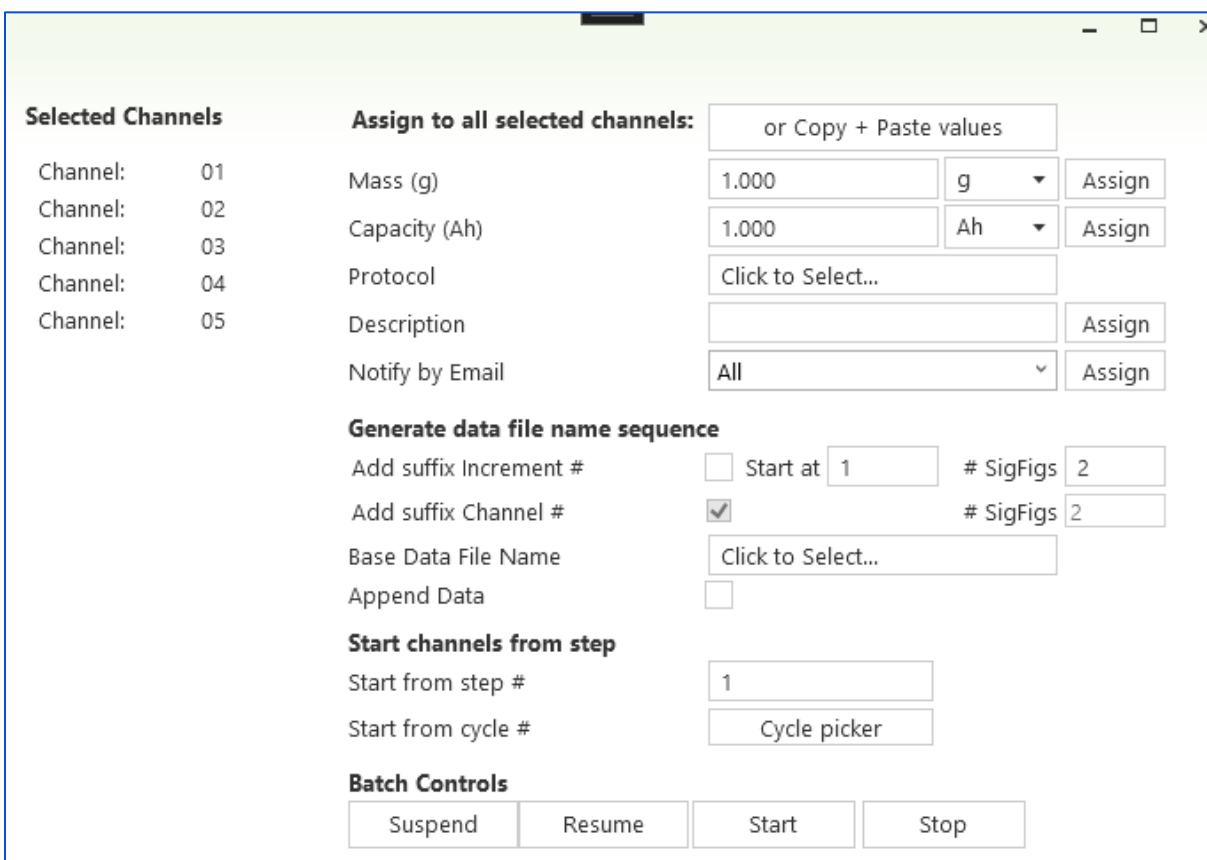

The screenshot shows a window titled "Batch Control" with a light green background. On the left, under "Selected Channels", there is a list of five channels (01 to 05) with their corresponding parameters: Mass (g), Capacity (Ah), Protocol, Description, and Notify by Email. To the right, under "Assign to all selected channels:", there are input fields for each parameter. The "Mass (g)" and "Capacity (Ah)" fields have "1.000" entered and unit dropdowns set to "g" and "Ah" respectively. The "Protocol" field has a "Click to Select..." button. The "Description" field is empty. The "Notify by Email" field has a dropdown set to "All". Each input field has an "Assign" button. Below this section, there is a "Generate data file name sequence" section with checkboxes for "Add suffix Increment #" (unchecked), "Add suffix Channel #" (checked), and "Base Data File Name" (with a "Click to Select..." button). There are also fields for "Start at 1" and "# SigFigs 2". Below that is a "Start channels from step" section with a "Start from step #" field set to "1" and a "Start from cycle #" field with a "Cycle picker" button. At the bottom, there is a "Batch Controls" section with four buttons: "Suspend", "Resume", "Start", and "Stop".

Figure 19: The batch control menu.

Mass to assign (g):

Entering a mass and clicking “Assign” will assign that mass to all selected channels.

Capacity to assign (Ah):

Entering a capacity and clicking “Assign” will assign that capacity to all selected channels.

Protocol to assign:



Clicking on the protocol file label (“Click to Select...”) will bring up file selector window, allowing a protocol file to be selected. Clicking “Assign file” will assign the specified protocol file to all selected channels.

Description:

Visual text for the description field of all selected channels. Also saved to test metadata.

Notify by Email:

Can select individual users, all, or no users to receive email notifications for all selected channels based on configuration in System Settings -> Email Notifications. Hidden when email notifications are not set up.

Generate a data file name sequence:

The batch control panel can be used to automatically assign sequential data file names to the selected channels. Clicking on the base file name label (“Click to Select...”) will bring up a file dialog where you can select the base file name to use.

The check boxes beside “Add suffix Increment #” and “Add suffix Channel #” determine what to append to the base file name. Suffix increment # will add a number to the end of the base file name, while the suffix channel # will add the channel number as shown in the channel control panel.

The “start at” box determines the number to append to the data file of the first channel in the selected channels list. The “# SigFigs” box determines the number of significant digits to display.

As an example, with a base file name of “c:\UHPC data\Cell Sequence.csv,” selecting “Add suffix Increment #,” a “# SigFigs” value of 2 will assign the following file names to the channels in the Selected Channels List when the “Assign” button is clicked:

C:\UHPC data\Cell Sequence-01.csv

C:\UHPC data\Cell Sequence-02.csv

C:\UHPC data\Cell Sequence-03.csv

C:\UHPC data\Cell Sequence-04.csv

C:\UHPC data\Cell Sequence-05.csv

The buttons at the bottom of the batch control panel are used to start, stop, suspend, resume the selected channels.

Append Data:

When checked, data will be written at the end of the file. No header lines will be written.



Cycle Picker:

The user can choose to start the channels from a specific step number or pick the spot in the cycle to start from. Selecting the “Cycle Picker” button will prompt the user with the protocol step list display (see *Figure 18*) in the Protocol Step List Panel section) where they can pick the spot directly from the list on where to start.

Or Copy + Paste Values:

Clicking Ctrl+V from the main UHPC Control channel grid or Clicking “Or Copy + Paste Values” button in batch control will open a batch control window that allows the user to batch enter unique values for each selected channel.

The format, seen below, allows for direct copy paste from excel columns.

The data entered must be in the column format seen below, with rows matching the number of selected channels.

Clicking Return to Main Page will switch back to the Batch Control window.

Selected Channels

Channel: 01
Channel: 02
Channel: 03
Channel: 04
Channel: 05

Return to Main Page

This form is for copy pasting a column from excel to batch assign unique values, and may be accessed quickly from the channel grid with Ctrl+V after selecting channels. Ensure the number of rows matches the number of selected channels. Please see the Batch Control section of the user manual for additional explanation and formatting.

1.5
1.6
1.54
1.42
1.5

Assign Capacity	Assign Mass	Assign Area
Assign Cell ID	Assign DataFile Name	

Figure 20: The batch control copy-paste window.

5.1.7 Startup Configuration

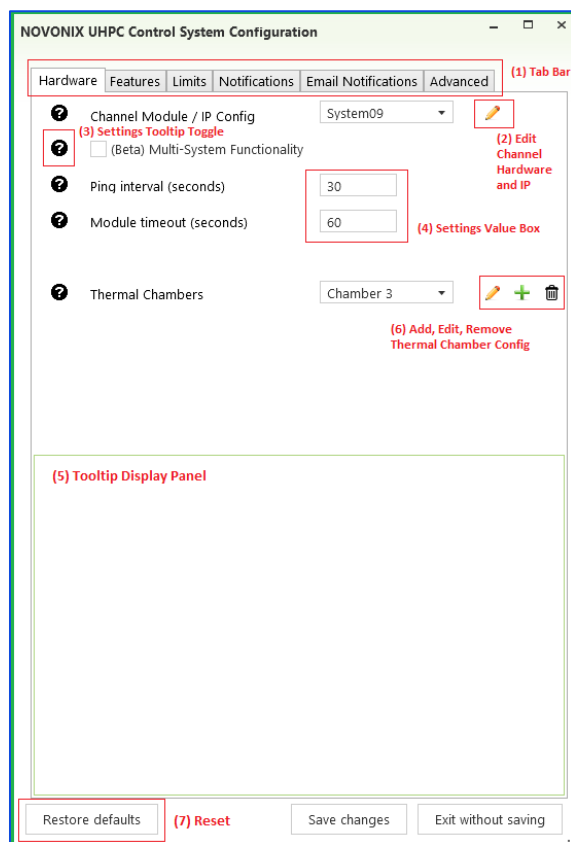


Figure 21: Startup configuration menu.

Tab Bar (1):

Switch between general settings and extra features menus.

1. Hardware & Feature Tabs:
 - a. Adjust operator preferences in the configuration of UHPC. Click the “Setting Tooltip Toggle” beside an option for more information on each.
2. Notifications Tab:
 - a. Manage popups and user preferences during UHPC Control operation.
3. Email Notifications Tab:
 - a. Manage email notification settings on UHPC channel status changes.
4. Advanced Tab:
 - a. Administrator settings typically for enhanced control during beta feature development and higher risk user functionalities.

Edit Channel Hardware and IP (6):

Clicking this will open a window for the user to set the system name and IP of their master controller, as well as number of channels per system and type of system (2A, 10A, 20A).

**Setting Tooltip Toggle (3):**

Clicking here displays detailed information for that setting in the tooltip display panel.

Settings Value Box (4):

Input area to change the value of the setting directly to its left.

Tooltip Display Panel (5):

Tooltip information is displayed here to explain the setting directly to its right.

Add, Edit, Remove Thermal Chamber Config (6):

Click this will open a window for the user to configure individual connected IP-enabled Thermal chambers. For more information see [Appendix A – Temperature Control](#).

Reset Configuration (7):

Clicking this will prompt the user to reset *all* UHPC Control Configurations to default values. A software restart is recommended to ensure all default values take effect.

[5.1.8 Diagnostics](#)

The Diagnostics page, seen below in *Figure 22*, is to help the user troubleshoot the system, and aid in customer support.

Troubleshoot Network:

This button begins a network diagnostic test to try and determine the IP of the UHPC Hardware and establish a connection if possible.

The two default IPs are “172.29.9.1” and older systems may be “192.168.1.1”.

If the system is turned on and properly connected and this test fails to establish a connection, the issue is that the PC hasn’t been configured properly. See section [First Time PC IP Address Setup](#) or [contact us](#) for network configuration details.

Flashing LED Test:

Clicking this button will flash the LED on the connected UHPC Channel Module(s). The “CH: All” dropdown box can be clicked to choose a specific channel. The channel(s) selected will flash for 30 seconds before the test halts.



Generate Diagnostics Report:

This is used to generate a diagnostic report containing the characteristics of connected UHPC hardware. This report may be requested by Avrion customer support when troubleshooting UHPC issues. This report takes several minutes to complete. When complete, a button “Open Latest Report” will also appear beside “Clear Log”.

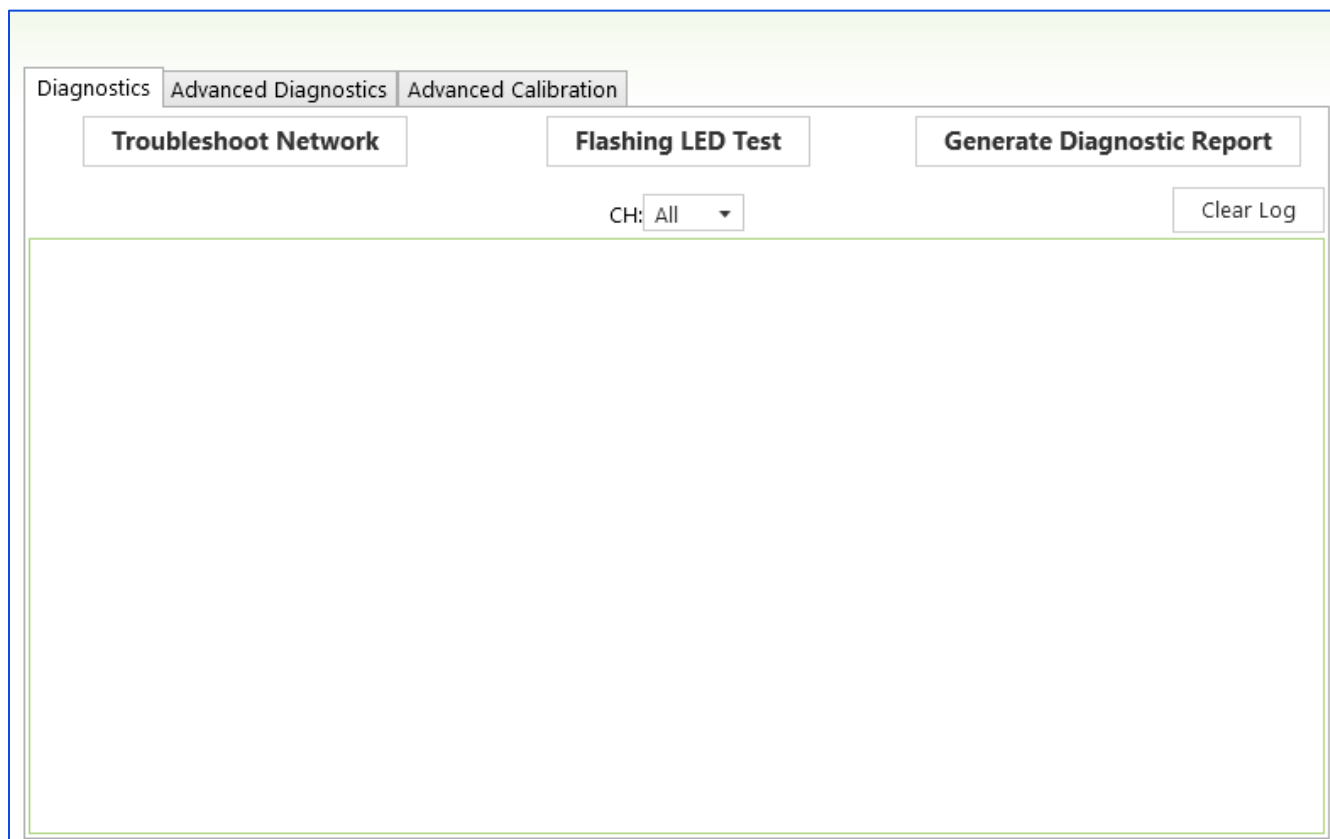


Figure 22: Diagnostics Panel


Advanced Diagnostics

The Advanced Diagnostics panel is available only to administrative users. Its intended purpose is to aid in Avrion customer support directly working with users to troubleshoot and resolve system issues.

Advanced Calibration

The Advanced Calibration panel is available to administrative users and certified third-party calibrators. Its intended purpose is to set calibration coefficients through software and help ensure the accuracy of the UHPC system.

5.1.9 Column Configuration

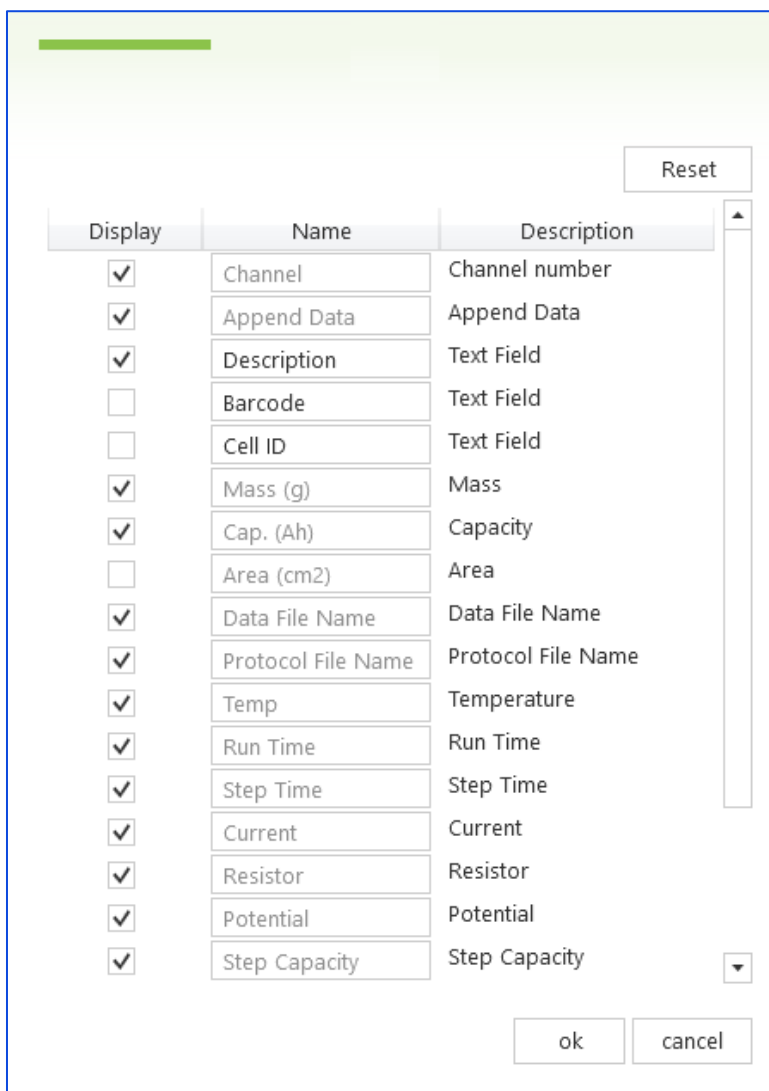

Display	Name	Description
☒	Channel	Channel number
☒	Append Data	Append Data
☒	Description	Text Field
☐	Barcode	Text Field
☐	Cell ID	Text Field
☒	Mass (g)	Mass
☒	Cap. (Ah)	Capacity
☐	Area (cm2)	Area
☒	Data File Name	Data File Name
☒	Protocol File Name	Protocol File Name
☒	Temp	Temperature
☒	Run Time	Run Time
☒	Step Time	Step Time
☒	Current	Current
☒	Resistor	Resistor
☒	Potential	Potential
☒	Step Capacity	Step Capacity

Figure 23: Column configuration menu.

Display:

Controls whether a column will be displayed or not (this will not affect what is being saved to the data file).

Name:

The title of the column. Only some columns can be edited.

Description:

The description of the column. This is a non-editable field.

5.1.10 Safety Limits

This window displays the maximum and minimum values that are allowed while running cells. Clicking the edit button will prompt a password dialog. Only those with a password can change the limits. Changing the global limits to values more restrictive could cause channels to shut down if the limits are passed.

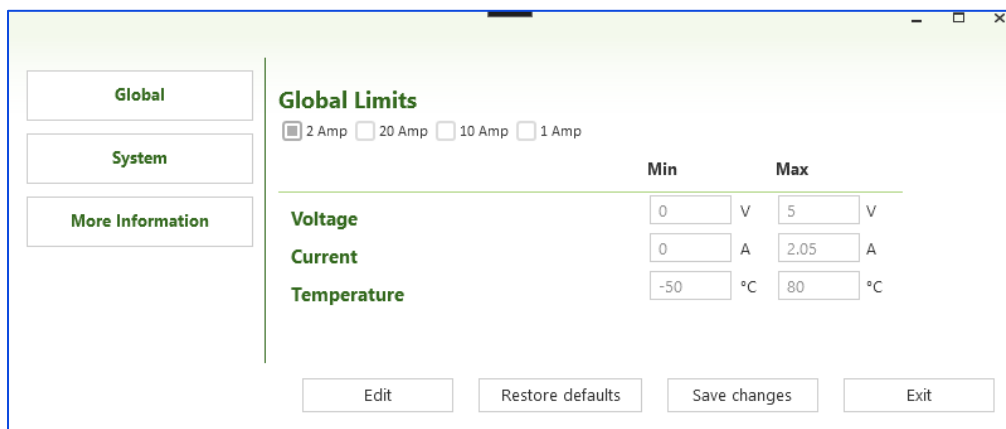


Figure 24: Safety limits menu, showing the default global limits view.

5.1.11 Restart from Previous Snapshot Data

Click the “Restart from previous channel snapshot” to bring up a list of saved snapshots. The list of snapshots represents the snapshot that is being written every second a channel is running. Archived snapshots are saved on a time-based interval which is defaulted to 1 hour.

Select the snapshot(s) you wish to start running again (you can hold down the left mouse button and drag or use ctrl to single click multiple entries). To complete this process, click “Load Selected Snapshots.”

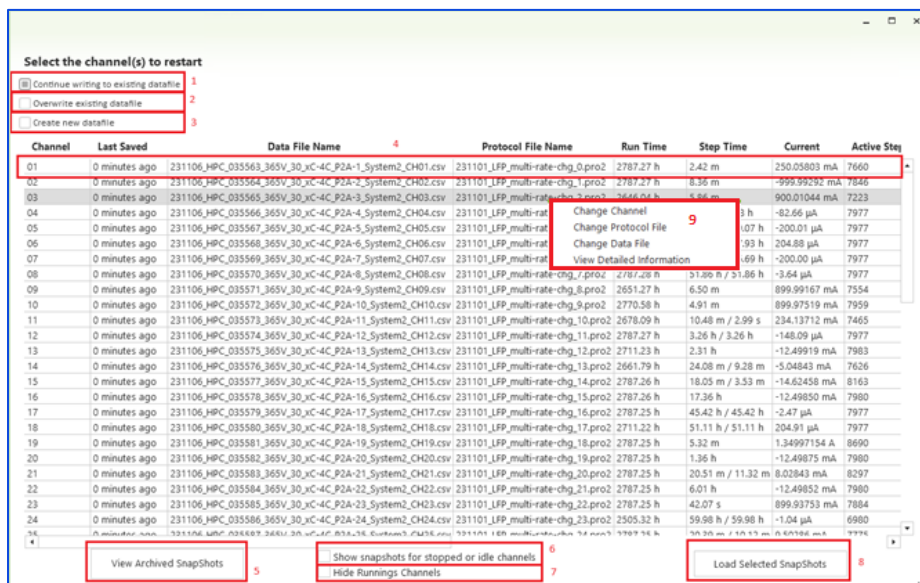


Figure 25: Menu to select specific snapshots to start.



Continue Writing to Existing Datafile (1):

The default option, clicking this radio button will cause restarted snapshots to resume writing from where they left off in the datafile.

Overwrite Existing Datafile (2):

Clicking this radio button reuses the existing datafile but erases all previous data.

Create New Datafile (3):

Clicking this radio button creates a new datafile for each snapshot when restarted. Previous data will not be included in the file. The new filename will be the previous file name with a timestamp appended on the end in the format of “-yyyy-MM-dd_HHmm.”

Snapshot list Channel Grid (4):

Snapshot details per channel will be listed in the grid, and channels can be selected individually with left mouse click, or in groups with shift/ctrl+click.

Right clicking a channel result in a dropdown, shown below in Figure 26. Change Channel can be used to move a snapshot to another channel. Protocol and datafile can be edited, and additional snapshot information can be seen with “View Detailed Information.”

Warning: Changing the protocol file can result in unintended consequences. In these cases, it’s best to immediately examine the channel upon restart and ensure the step is loaded correctly. “Suspend” + “Jump to step” from the channel protocol description may be helpful in these situations.

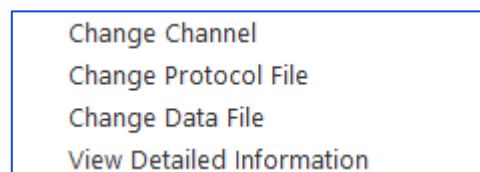


Figure 26: Snapshot Channel Right Click Dropdown

View Archived Snapshots (5):

This button will change the dialog screen to a list of archived snapshots. These “snapshots” of snapshots are taken once every hour while tests are running and are stored for up to 2 months. Each list will represent the state of the system at the time of the archived snapshot state. Selecting an archived snapshot list or selecting latest running snapshot for each channel will reload *Figure 25* with the snapshots at that time. Resuming snapshots from the past may result in datafiles with inconsistent timestamps or repeat previous steps.

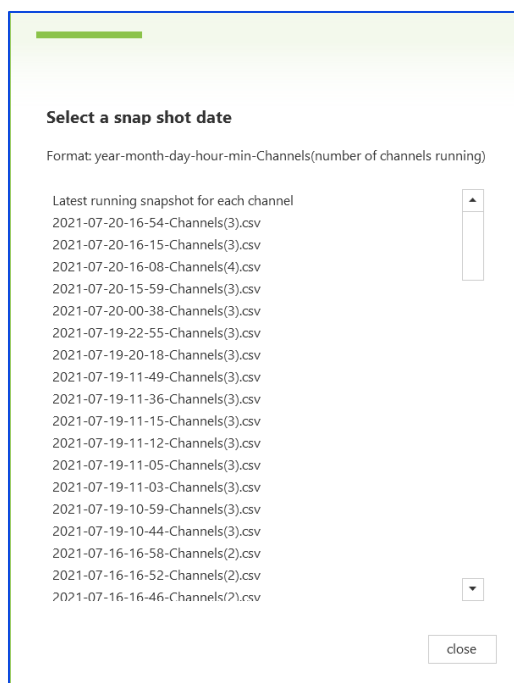


Figure 27: Initial snapshot date choice menu.

Show snapshots for stopped or idle channels (6):

By default, stopped channels are not displayed on this list, only channels that were running when the software was shut down (unless all channels were stopped at once). Similarly, if a user restarts only a portion of the channels with snapshot, the remaining channels will be marked as idle and hidden as well. The intent is that only the most active channels should be displayed to be restarted from snapshot, rather than displaying all channels all the time. Clicking this checkbox will display all previously stopped and idle channels.

Hide Running Channels (7):

Running channels are displayed by default, primarily so that users can see that snapshots are actively being recorded. If restarting idle channels while other channels are running, clicking this checkbox will hide active channels, only displaying the remaining channels. This checkbox should be used in conjunction with “show snapshots for idle/stopped channels.”

Load Selected Snapshots (8):

When snapshot(s) have been selected with the left mouse button (or ctrl/shift click to select multiple snapshots), clicking this button will begin the process to restart all selected channels from snapshot.

Right Click Menu (9):

When a single snapshot has been selected, and the right click button pressed. A dropdown menu will appear allowing the user to change the channel the snapshot is assigned to, as well as changing the datafile, protocol file, and some detailed information about the snapshot.

Warning: When changing the protocol file, the snapshot will resume on the same step number it left off on, this can result in unintended behavior if the steps have been reordered or reduced.

5.1.12 Temperature Linking

Temperatures can be linked between channels by selecting two or more channels, then right-clicking and selecting Link Temperature(s).

Protocol File Name	Temp
Batch Control	33.001°C
Clear Cell	43.001°C
Clear Selected Rows	53.001°C
Reset Selected Rows	63.001°C
Deselect Row(s)	---
Link Temperature(s)	---
Un-link Temperature(s)	---
Link Voltage(s)	---
Un-link Voltage(s)	---

Figure 28: The right-click menu showing the Link Temperature(s) option.

The anchor is the channel that copies its temperature to the other channels. The color will display will indicate which channel is the anchor.

Which channel would you like to be the anchor?

Select the color to represent the link

Figure 29: The temperature assignment menu.

Temp
32.999°C
32.999°C
32.999°C
32.999°C

Figure 30: Linked temperatures as assigned by the previous box. The anchor channel is the topmost channel.

5.1.13 Voltage Linking

Voltages can be linked by selecting two or more channels, right-clicking, and selecting the Link Voltage(s) option. Note that only Idle channels can be assigned voltage links.

	Step Time	Current	Potential
			2.000054 V
Batch Control			2.000054 V
Clear Cell			2.000054 V
Clear Selected Rows			2.000054 V
Reset Selected Rows			2.000054 V
Deselect Row(s)			2.000054 V
Link Temperature(s)			2.000054 V
Un-link Temperature(s)			2.000054 V
Link Voltage(s)			2.000054 V
Un-link Voltage(s)			2.000054 V

Figure 31: The right-click menu showing the Link Voltage(s) option.

Unlike temperature links, voltage links involve the use of a reference as well as a base channel.

- The base channel saves the voltage data from all other connected channels along with its own output data.
- When the base channel has a protocol that checks the “ref voltage” value, it checks the voltage of the reference channel and performs the step operation based on that value (rather than its own voltage).
- Non-base, non-reference channels have their voltage data saved along with the base channel’s.

Which channel would you like to be the base?

Which channel would you like to be the reference?

Select the color to represent the link

Figure 32: Menu prompting for a base, reference, and representative colour for the new link.

5.1.14 Snapshots with Voltage and Temperature Links

Snapshots cannot be imported onto channels with existing temperature or voltage links, or channels that are not in the Idle state. Attempting to import onto a channel with links or that is running will not succeed.

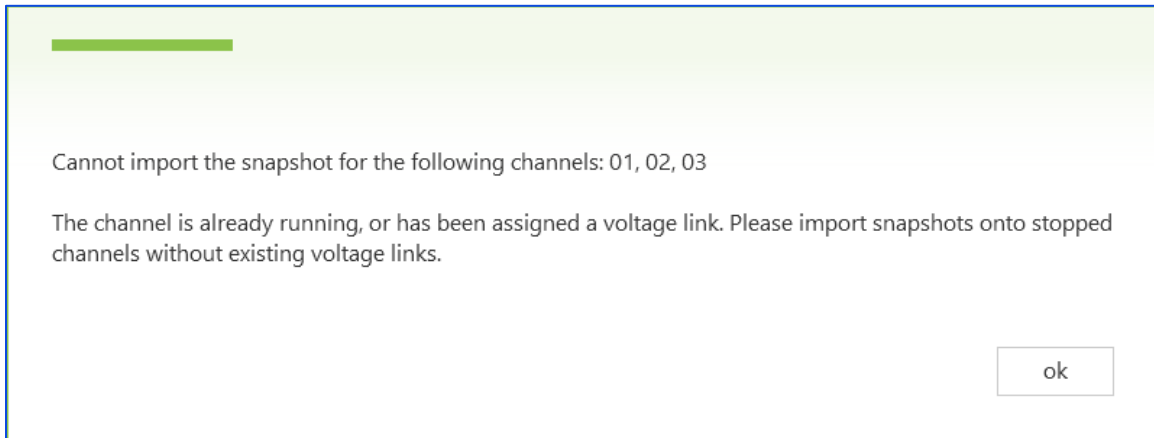


Figure 33: Notification showing user cannot perform the requested action.

If the colour assigned to the temperature or voltage links of the snapshot channel is already in use by a channel in the program, the program will dynamically re-assign a colour to the imported snapshot channel. If this is not possible, the program will display an error.

6. UHPC Protocol Software Designer Manual

6.1 Main Protocol Software Operation

The protocol designer software is used to develop a test protocol to be used with the UHPC Control program. The test protocol details the sequence of test steps to be performed on a cell. A given protocol file can be used for multiple channels.

When you first start the protocol designer software, you will be prompted to select the channel type to develop a protocol for (e.g., 2 A UHPC channels or 20 A UHPC channels).

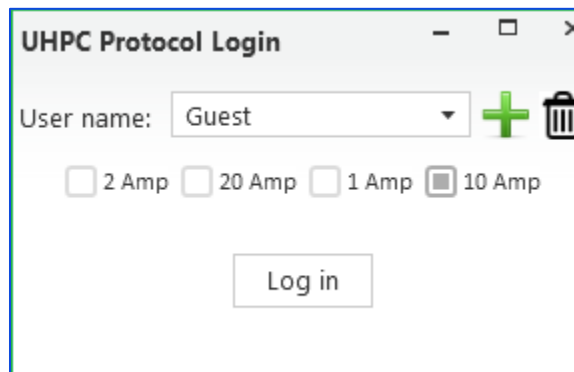


Figure 34: The UHPC Protocol login prompt.

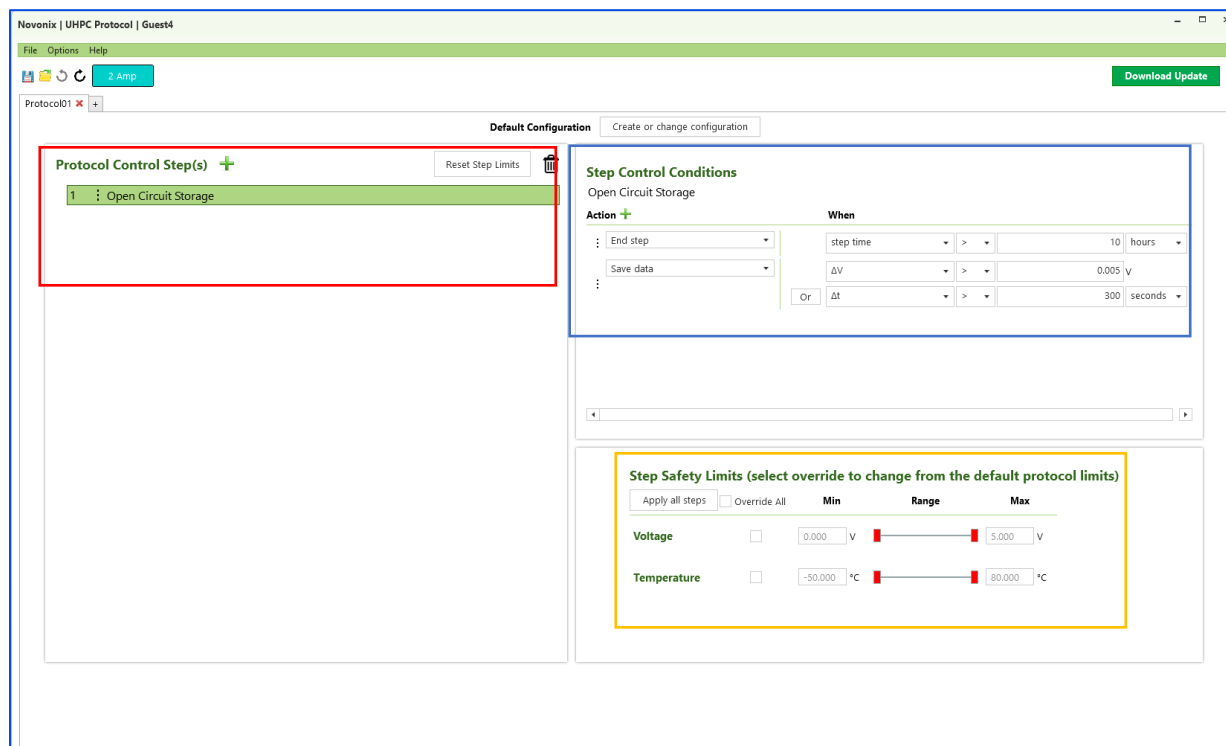


Figure 35: The main screen of the program when first loaded.

6.1.1 Control Options

Protocol Control Step(s) + 🗑️

1	⚙️	Repeat steps below	2	times	
2	⋮	Open Circuit Storage			
3	⋮	Constant Current Charge	1	A ▼	to 4.2 V
4	⋮	Constant Current Discharge	1	A ▼	to 2.8 V
5	⋮	CC-CV Charge	1	A ▼	to 4.2 V
6	⋮	CC-CV Discharge	1	A ▼	to 2.8 V
7	⋮	Increment Cycle Counter			

Figure 36: Each of the protocol control step options with their default values.

Open Circuit Storage:

This will measure open circuit voltage as a function of time for a fixed storage period specified by the user in the trip condition. Data will be saved when the open circuit voltage changes by a fixed amount specified by DV (e.g., 0.005 V) or when a fixed time interval passes, specified by Dt (e.g., 5 minutes). These two parameters are not mutually exclusive - data will be saved when either parameter is reached and then the start point for the next data interval will be reset for both parameters.

Constant Current Charge:

The cell will be charged at constant current (specified by the user) to a voltage limit. A time trip condition is also recommended. Typically, this period is used to be longer than the time expected for the cell to charge and acts as a safety limit. For example, if a C/20 charge is used with a 25-hour time trip and the cell develops a short and does not reach the voltage trip point after 25 hours, it will move to the next step.

The following units are available for the current:

- A, mA, μ A: current will be in the specified absolute units. The current is restricted to the range 1 μ A to 1A.
- A/g, mA/g, μ A/g: These units are designed to be used when an active mass is entered in the control program.
- xx-C, C/xx: These units are designed to be used when a cell needs to be charged at a particular C-rate. The values would be coupled with the cell capacities entered in the main control program. If 2 is entered in the numeric field for xx-C units, this indicates a 2-C rate. If 2 is entered in the numeric field with the C/xx units, this indicates a C/2 rate.

Constant Current Discharge:

The cell will be discharged at constant current (specified by the user) to a voltage limit. A time trip condition is also recommended. Typically, this period will be longer than the time expected for the cell to discharge; it then acts as a safety limit should, for example, the cell develops a short and not



reach the voltage trip point.

CC-CV Charge:

This step control type will charge the cell at constant current to the specified voltage limit and then hold the cell at that voltage for a period. The constant current (maximum charge current) and the hold voltage to be used are both entered by the user. When the voltage reaches this limit, the current will gradually reduce to maintain the cell at this voltage. The cell may slightly overshoot and then oscillate around the set-point before settling.

There are separate trip conditions for the overall and CV portions of the step. There are no specific trip conditions related to the CC portion of the step.

- The first trip condition will stop the step and move on to the next step if the TOTAL step time (CC + CV) exceeds the time entered by the user.
- The second trip condition will stop the step and move on to the next step if either the CV hold time exceeds the time entered or if the amperage of the measured current drops below the value entered by the user.

The same range of units available for the constant current control are available for the trip conditions on the constant voltage control.

CC-CV Discharge:

This step control type will discharge the cell at constant current to a voltage limit and then hold the cell at that voltage for a period. The constant current (maximum absolute discharge current) and the hold voltage to be used are both entered by the user. When the voltage reaches this limit, the amperage of the current will gradually reduce to maintain the cell at this voltage. The cell may slightly undershoot and then oscillate around the set-point before settling.

There are separate trip conditions for the overall and CV portions of the step. There is no specific trip conditions related to the CC portion of the step.

- The first trip condition will stop the step and move on to the next step if the TOTAL step time (CC + CV) exceeds the time entered by the user.
- The second trip condition will stop the step and move on to the next step if either the CV hold time exceeds the time entered or if the amperage of the measured current drops below the value entered by the user.

The same range of units available for the constant current control are available for the trip conditions on the constant voltage control.

Repeat Step(s):

This step control type allows steps to be placed in a loop. The steps to be repeated will appear identical to the repeat step as per Figure 34 above. The repeat count value indicates the total number of times the steps in the repeat block will be run (i.e., a value of 2 means that each step will be run 2 times). Multiple repeat steps can be included in a protocol and repeat steps can be repeated within other repeat steps, allowing for nested loops.



Increment Cycle Counter:

An increment cycle counter step needs to be explicitly added for each time you would like the control program to increase the cycle number. This gives you full control over how you wish to define a cycle, rather than having it defined in a way that may not work for your test needs. This control type has no trip or save conditions attached to it.

Set Temperature:

A Set Temperature step control type allows for temperature control of Avrion IP-Enabled thermal chambers. When the set temperature step starts, a command will be sent to the thermal chamber temperature controller associated with the running channel. The temperature will be set once, and then run until the end step conditions are met. Step control conditions are described below, but by default for Set Temperature; Temperature Variance and Temperature Hold control conditions are used. Which cause the Set Temperature step to end successfully when the chamber temperature is held at the set point within the variance tolerance for the total hold time. Unlike the normal “temperature” condition, which uses cell temperature, Temperature Variance and Temperature Hold use the thermal chamber temperature.

Because Set Temperature uses a specialized condition “Temperature Variance” where temperature is held at a specific value for a set amount of time, looking at *Figure 37* will provide the minimum Avrion recommended temperature variance values based on target temperature. The default value for Temperature Variance is set to 1C to stay within this band during most use cases.

Peltier Cooling Chamber Summary									
Rated Specs									
Temperature (°C)	10	15	20	30	40	50	60	70	80
Point Stability (°C)	±0.06	±0.02	±0.02	±0.02	±0.02	±0.04	±0.03	±0.05	±0.04
Accuracy (°C)	±1.3	±0.3	±0.2	±0.3	±0.7	±1.3	±1.1	±1.5	±1.9

Figure 37: Peltier Chamber Accuracy based on Temperature

EIS:

An EIS step control type allows for Electrochemical Impedance Testing (EIS) through use with a connected Gamry EIS module. Once an EIS step type is selected, the operator can choose from three types of EIS testing.

Potentiostatic: The most commonly used EIS test, Potentiostatic mode is used when maintaining a constant voltage is crucial. This mode is ideal for studying the electrode processes and battery cell behavior at a fixed potential, making it useful for analyzing the stability and efficiency of the cell under a specific voltage. Researchers often employ this mode to understand the reaction kinetics and to identify the resistive and capacitive elements within the cell.

You wouldn't want to run a test in Potentiostatic mode if the impedance of the cell is very high, as

this could result in unstable voltage control and inaccurate measurements.


Galvanostatic: Galvanostatic mode is employed when a constant current is required during EIS testing. This mode is particularly useful for examining the response of a battery cell to steady current flow, which is representative of real-world operating conditions. It allows for the study of charge transfer resistance and mass transport processes, making it valuable for understanding the performance and limitations of the battery under consistent load.

Avoid using galvanostatic mode if the cell has very low impedance, as maintaining a constant current can lead to excessively high or low voltages that may damage the cell or distort the data.

Hybrid: Hybrid mode combines the features of both potentiostatic and galvanostatic modes, allowing for more versatile and comprehensive EIS testing. This mode can adapt to changing conditions by switching between maintaining a constant voltage or current as needed. It is beneficial for dynamic studies where the battery cell's behavior under varying loads and potentials needs to be analyzed, providing a more complete understanding of the cell's electrochemical characteristics.

Hybrid mode may not be ideal if the system's response is highly non-linear, as the switching between voltage and current control could introduce artifacts or complicate the interpretation of the impedance data.

As seen below in *Figure 38*, after selecting which EIS mode to run in, clicking “Configure” will open a configuration dialog for that EIS step. **Please note:** EIS values are not all validated by UHPC at this time, when creating a new EIS configuration, follow the Gamry recommend value ranges for your EIS device and testing scenarios.

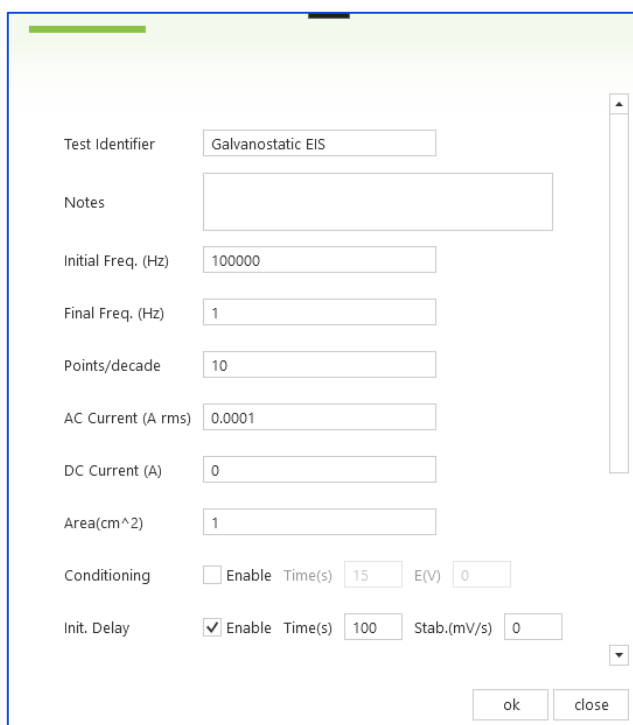

Test Identifier	Galvanostatic EIS		
Notes			
Initial Freq. (Hz)	100000		
Final Freq. (Hz)	1		
Points/decade	10		
AC Current (A rms)	0.0001		
DC Current (A)	0		
Area(cm^2)	1		
Conditioning	☐ Enable	Time(s) 15	E(V) 0
Init. Delay	☒ Enable	Time(s) 100	Stab.(mV/s) 0

ok close

Figure 38: Configure EIS (Galvanostatic) Step Type

For more information, please check the attached [Appendix B – Gamry EIS Integration](#).

6.1.2 Control Conditions

The control conditions show the logical representation on what action will happen when the conditions are fulfilled. Actions can be added by clicking the green + icon or by using the right click menu. Conditions can also separately be added or removed by the right click menu.

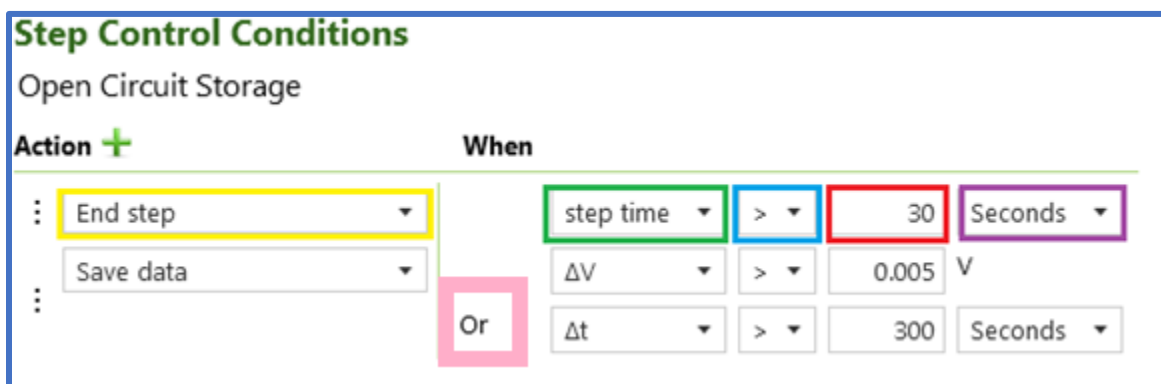


Figure 39: Step control conditions, with each important segment highlighted.

Action:

Highlighted in yellow, the action represents what the channel should do when its “when” condition is satisfied. The options for the action control are:

- End step, which ends the currently running step and proceeds to the next (if available),
- End protocol, which jumps to the end of the protocol and sets the channel status to completed,
- Pause protocol, which suspends the channel until it is manually resumed,
- End loop, which exits the current loop and continues to the next step outside the current loop (if available), and
- Save data, which saves channel information to the step’s data file.

AND / OR:

Highlighted in pink, the “And/Or” represents how the conditions are treated as a group. If a set of conditions are set to “And” then all grouped conditions must be met simultaneously before that corresponding action is taken. Alternatively, if “Or” is selected, any met condition will trigger the corresponding action.

Left side condition:

Highlighted in green, the left side condition is the left side of the condition’s comparison. It acts as the condition to be checked against, generally a unit or function of a unit(s).

Abbreviations for table below:

- CC = Constant Current
- CC-CV = Constant Current-Constant Voltage
- OCS = Open Circuit Storage
- Ch = Charge
- Dc = Discharge
- ST = Set Temperature

All left side conditions available in the program are as follows:

Condition	Suitable for Use On	Description
ΔV	OCS: Save data CC Ch & Dc: Save data CC-CV Ch & Dc: Save data during CC, save data any time	Saves when the voltage has changed from its last save point value by the amount specified in the condition.
Δt	OCS: Save data CC Ch & Dc: Save data CC-CV Ch & Dc: Save data (all)	Saves when the time elapsed has changed from its last save point value by the amount specified in the condition.
ΔI	CC Ch & Dc: Save data CC-CV Ch & Dc: Save data during CV, save data any time	Saves when the current has changed from its last save point value by the amount specified in the condition.
ΔQ	CC Ch & Dc: Save data CC-CV Ch & Dc: Save data (all)	Saves when the capacity has changed from its last save point value by the amount specified in the condition.
Abs(dV/dt)	OCS: All (except save data) CC-CV Ch & Dc: All (except save data) any time, all (except save data) during CC	Saves when the absolute value of ($\Delta V/\Delta t$) hits the specified value.
Abs(dI/dt)	CC-CV Ch & Dc: All (except save data) any time, all (except save data) during CV	Saves when the absolute value of ($\Delta I/\Delta t$) hits the specified value.
Abs(I)	CC-CV Ch & Dc: All (except save data) any time, all (except save data) during CV	Saves when the absolute value of the current (I) hits the specified value.
Step time	OCS: All (except save data) CC Ch & Dc: All (except save data) CC-CV Ch & Dc: All (except save data)	Trips when step time for the channel reaches the specified value.
Hold time	CC-CV Ch & Dc: All (except save data) any time, all (except save data) during CV	Trips when the voltage has been held for the specified length of time.
Temperature	OCS: All (except save data) CC Ch & Dc: All (except save data) CC-CV Ch & Dc: All (except save data)	Trips when the channel temperature reaches the specified value.
Voltage	OCS: All (except save data) CC Ch & Dc: All (except save data) CC-CV Ch & Dc: All (except save data)	Trips when the channel voltage reaches the specified value.
Reference voltage	OCS: All (except save data) CC Ch & Dc: All (except save data) CC-CV Ch & Dc: All (except save data)	Trips when the reference voltage reaches the specified value. This only applies on base channels. See UPHC Control manual for more information on base and reference voltages.



Cumulative Capacity	CC Ch & Dc: All (except save data) CC-CV Ch & Dc: All (except save data)	Trips when the channel cumulative capacity reaches the specified value.
(%) Cumulative Capacity	CC Ch & Dc: All (except save data) CC-CV Ch & Dc: All (except save data)	Trips when the channel cumulative capacity percentage reaches the specified value. Requires capacity to be set in UHPC Control program to function correctly.
Step Capacity	CC Ch & Dc: All (except save data) CC-CV Ch & Dc: All (except save data)	Trips when the channel step capacity reaches the specified value.
(%) Step Capacity	CC Ch & Dc: All (except save data) CC-CV Ch & Dc: All (except save data)	Trips when the channel step capacity percentage reaches the specified value. Requires capacity to be set in UHPC Control program to function correctly.
Temperature Variance	ST: All (except save data)	Trips when the chamber temperature is within the specified value range of assigned thermal chamber. See <i>Figure 39</i> for minimum recommended temperature variance.
Temperature Hold	OCS & ST: All (except save data)	Required Temperature Variance step, when paired, hold time begins when chamber temperature variance is stabilized.

Highlighted in **blue**, the comparator is the selection on what the comparison relationship that needs to be fulfilled to satisfy the condition. The > symbol denotes that the left side condition is *greater than* the right-side condition; the < symbol denotes the left side condition is *less than* the right-side condition. Note that some left side conditions can only use one type of comparator. A +/- comparator exists for the Temperature Variance condition.

Right side condition:

Highlighted in **red**, the right-side condition is the right side of the comparison. The right-side conditions are user defined and input into the text box as shown in *Figure 39* above.

Right side units:

Highlighted in **purple** is the selector for the units of the right-side condition. The units are associated with the left side condition. They may be set to one specific value (in which case they are expressed in plain text and not a drop-down box) or changeable by the user (as shown in *Figure 39* above).

6.1.3 Step Safety Limits

For each step created, there are optional safety limits that can be added. The default values for the step safety limits are derived from the protocol limits. To change these values to be more restrictive, click on the override checkbox beside the safety limit label (shown below highlighted in red).

Step Safety Limits (select override to change from the default protocol limits)

☐ Override All

Min

Range

Max

Voltage	<input style="border: 2px solid red;" type="checkbox"/>	0.000 V		5.000 V
Current	☐	0.000 A		2.050 A
Temperature	☐	-50.000 °C		80.000 °C

Figure 40: The step safety limits, with override box highlighted in red.

Apply all steps:

Copies all the limits as specified by the user to all other steps in the protocol, where applicable.

6.1.4 Step Manipulation

Selecting the green + icon will add a step underneath whatever step is currently selected. The “trash can icon” is used to delete any steps that are selected. Extended step manipulation options are also available from the drop-down menu that appears when right clicking on a control or condition step.

The available button/options are:

Add Step:

This will insert a new step above the currently selected step. If a step within a repeat block is selected, then this will insert a new step inside the repeat lock above the selected step. If a repeat step is selected, then this will insert a new step above the repeated step.

Loop items:

This will insert the currently selected step into a newly created “Repeat steps below” step.

Copy:

Copies the selected step(s).

Paste before:

If there are step(s) that have been copied, this command will insert the copied step(s) above the currently selected step.

Paste after:

If there are step(s) that have been copied, this command will insert the copied step(s) below the currently selected step.

Delete:

This will delete the currently selected step(s).

There is additional functionality outside the right-click menu, described below:

Drag and drop:

Users can move steps around by clicking while holding the mouse button down and then dragging above below or into a loop.

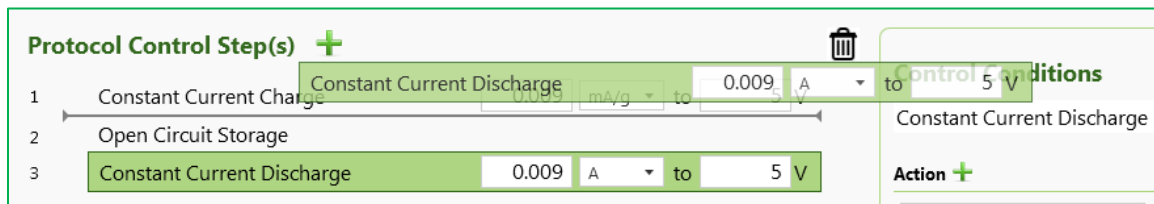


Figure 41: Dragging a step.

Change step type:

Users can change the step into a different step by double clicking on the step's name. A dialog will open prompting the user to select the type of step they wish to change their selection to.

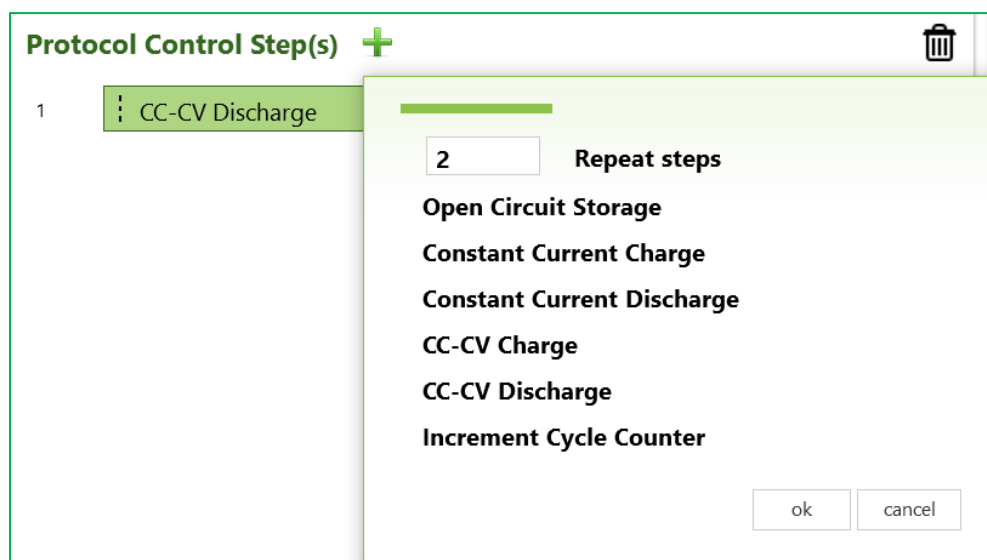


Figure 42: The step selection menu, pulled up by double-clicking the "CC-CV Discharge step."

6.1.5 Menu Options

File Menu:

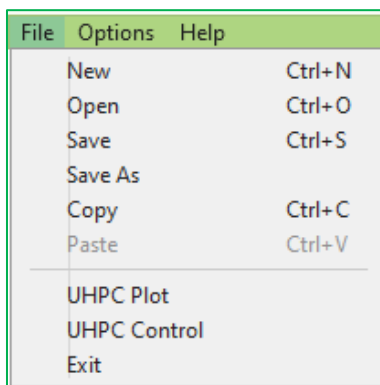


Figure 43: The File drop-down menu.

New (Ctrl+N):

Creates a new protocol file, which is then displayed in the protocol tabs area.

Open (Ctrl+O):

Opens an existing protocol file for modification.

Save (Ctrl+S):

Saves the currently selected protocol file to the default file location, with its currently assigned name.

Save As:

Saves the currently selected protocol file to a new location and/or with a new name.

Copy (Ctrl+C):

Copies the currently selected protocol control step(s) or step control condition(s).

Paste (Ctrl+V):

Pastes the item(s) currently on the clipboard (items that were previously copied), if possible.

UHPC Control:

This launches the UHPC Control program, which is used to run control steps for channel(s) that are assigned a protocol file (*.pro1, *.pro2) made from this application.

UHPC Plot:

This launches the UHPC Plot program that is used to analyse the data files collected and generate summary data files for subsequent graphing with external programs such as Open Office®, Microsoft Excel®, Golden Software Grapher® etc. This program allows the user to view graphical representations of the data collected both when cells are running and after testing.

Exit:

This will prompt the user to save any unsaved protocol files that they wish to keep, then closes the program.

Options Menu

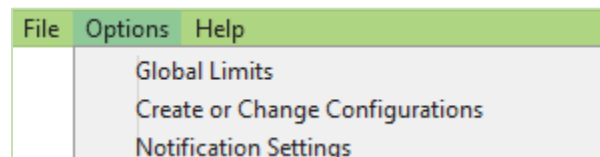


Figure 44: The Options drop-down menu.

Global Limits:

Opens the window for configuring global protocol safety limits. More information can be found in the [Global Limits](#) section below. Requires an administrator password from Avrion to access.

Create or Change Configurations:

Used to customize the default values for protocol control steps, step control conditions, and user management. More information can be found in the [Default Configurations](#) section below.

Help Menu

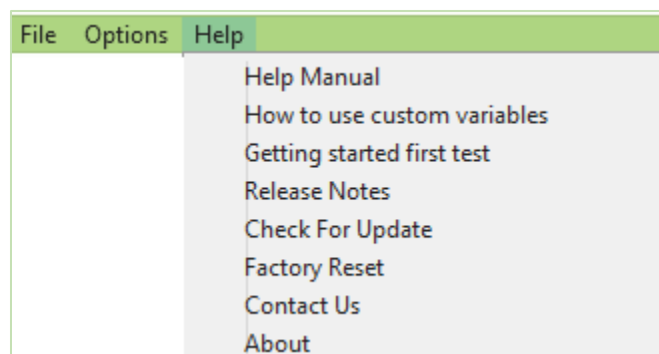


Figure 45: The Help drop-down menu.

Help Manual:

Launches the Help Manual for the HPC Protocol program (this document).

**How to use custom variables:**

Opens a PDF guide on utilizing custom variables to use advanced testing conditions.

Getting started first test:

Opens a PDF guide on conducting UHPC tests.

Check for update:

Checks the [Avrion Customer Portal](#) for available updates and then offers to download them. Requires network connection.

Factory Reset:

After suggesting all other UHPC applications are exited, removes all configuration files associated with UHPC Protocol, including Global Limits, System Limits, User Configurations, and saved application settings. Deleted files are those found in C:/AVRION.

Contact Us:

Provides the email address of [Avrion UHPC customer support](#).

About:

Provides information on the UHPC Protocol program.

6.1.6 Global Limits


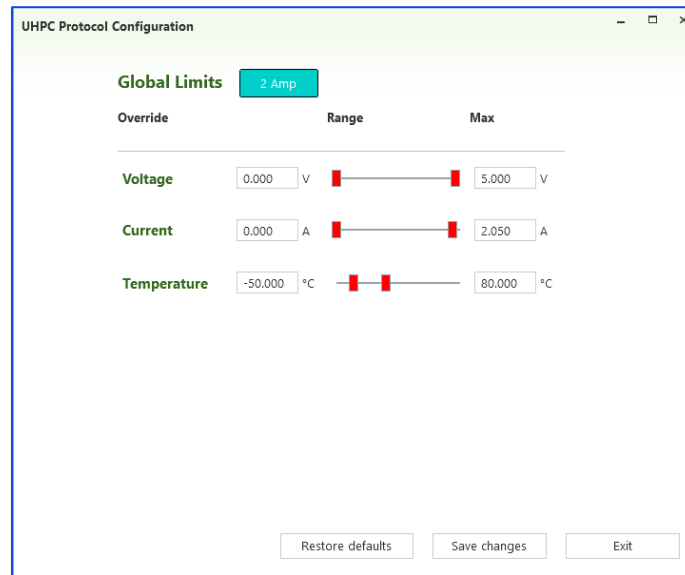


Figure 46: The Global Limits menu, as accessed by a supervisor account (fields can be edited).

Global limits are the safety limits set by an administrator role. To view/edit the rules, a supervisor password is required (or view them on UHPC Control). The maximum and minimum values for the bars are the system limits that are set in the control software. The default system limits are based off the channel type (2 Amp, 10 Amp, 20 Amp) chosen at start-up. These limits are also used as the default values for the step safety limits.

6.1.7 Default Configurations

The default configurations menu can be displayed both with the menu option (Options > Create or Change Configuration), or with the “create or change configuration” button displayed above the protocol control steps and step control conditions areas of the window.

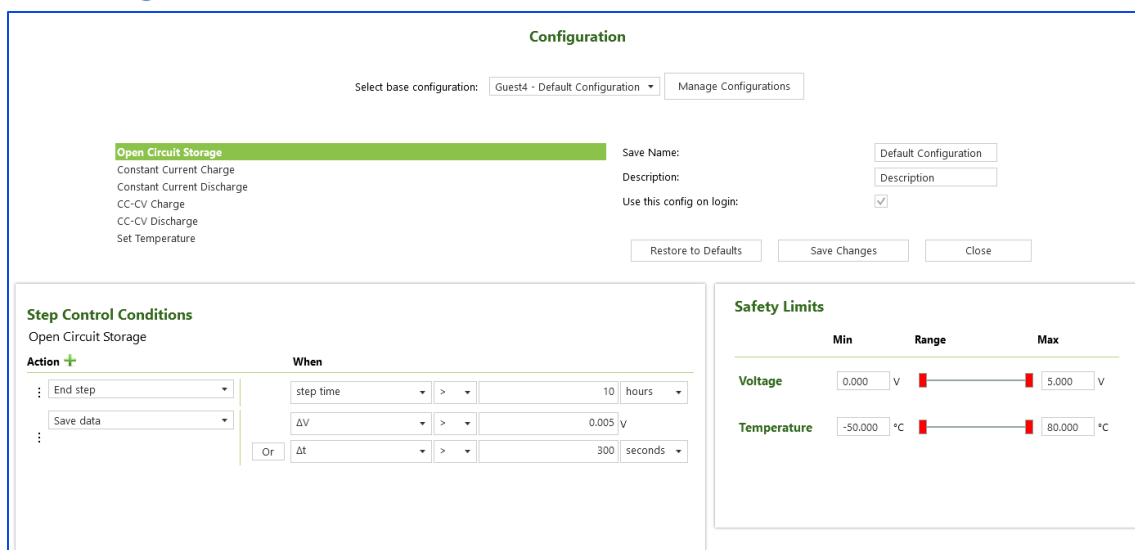

The screenshot shows the 'Configuration' window. At the top, it says 'Select base configuration: Guest4 - Default Configuration' with a 'Manage Configurations' button. Below this, a list of protocols is shown, with 'Open Circuit Storage' selected. To the right of this list, there are fields for 'Save Name' (Default Configuration), 'Description' (Description), and a checkbox for 'Use this config on login' (checked). Below these are buttons for 'Restore to Defaults', 'Save Changes', and 'Close'.

The 'Step Control Conditions' section for 'Open Circuit Storage' shows a table with two rows. The first row has 'End step' in the 'Action' column and 'step time' in the 'When' column, with a value of '10' and units of 'hours'. The second row has 'Save data' in the 'Action' column and 'ΔV' in the 'When' column, with a value of '0.005' and units of 'V'. Below this table is an 'Or' button and a row with 'Δt' in the 'When' column, with a value of '300' and units of 'seconds'.

The 'Safety Limits' section shows two rows. The first row is for 'Voltage' with a 'Min' value of '0.000' and a 'Max' value of '5.000', both in 'V'. The second row is for 'Temperature' with a 'Min' value of '-50.000' and a 'Max' value of '80.000', both in '°C'.

Figure 47: The configuration menu opened and showing the default values for the Open Circuit Storage protocol step.

Step Controls Conditions:

These areas function the same way as setting step control conditions and limits for an individual step inside a protocol. Selecting the step type will display the default conditions and safety limits associated with that step. In the image above Open Circuit Storage is selected, so the conditions and safety limits shown below are the defaults that will be used whenever a new Open Circuit Storage step is created with the configuration applied. (See Control Conditions section for more detail)

Saving Configurations:

To save a new configuration simply change the save name (defaults to “Default Configuration”) and click the “Save Changes” button. A new entry will be created and attached to the logged in username. Using different users’ configuration is permitted, however, saving changes will save the configuration under the username of the user who made the changes.

Exit Configuration:

To leave the Configuration screen, click the “Close” button.

Manage Configuration:

Click “Manage Configurations” to choose from a list of all configurations. Double click to select configuration. Right-click to bring up a context menu to either user or delete the configuration.

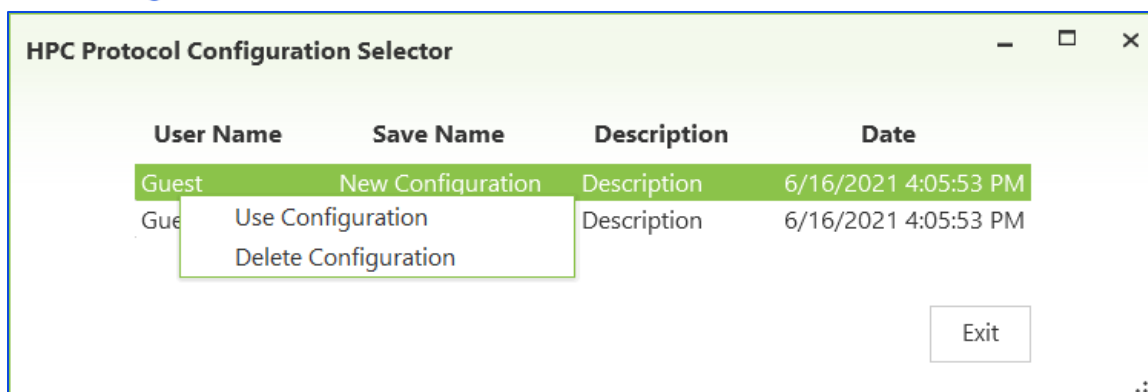


Figure 48: Configuration selector showing the “right-click” menu.

Default Configuration:

Click “Use this config on Login” to use the configuration as the currently logged in user’s default. The button will be disabled and be surrounded by a green square (as shown above) when it is currently the default configuration.

7. UHPC Plot Data Analysis Manual

7.1 UHPC Plot Software Operation

A graphical data viewing and analysis program has been included with the UHPC system. This program allows the user to view a range of plots for multiple cells and generate summary text-based data files for subsequent analysis through programs such as Microsoft Excel®, Golden Software Grapher®, etc. A shortcut can be found on the desktop and in the start menu under the Avrion folder.

It is important to understand that several of the values that can be plotted are calculated from the raw data files and that, in some instances, the UHPC Plot software uses internal algorithms to ensure the values are presented correctly. Care must be taken if you intend to work with the raw data files directly.

Starting up the application will prompt a file explorer window that will allow you to select the files you wish to analyse first. If you select ‘cancel,’ no graphs will be shown on the main page; however, you can still choose to add more files once the main screen is shown.

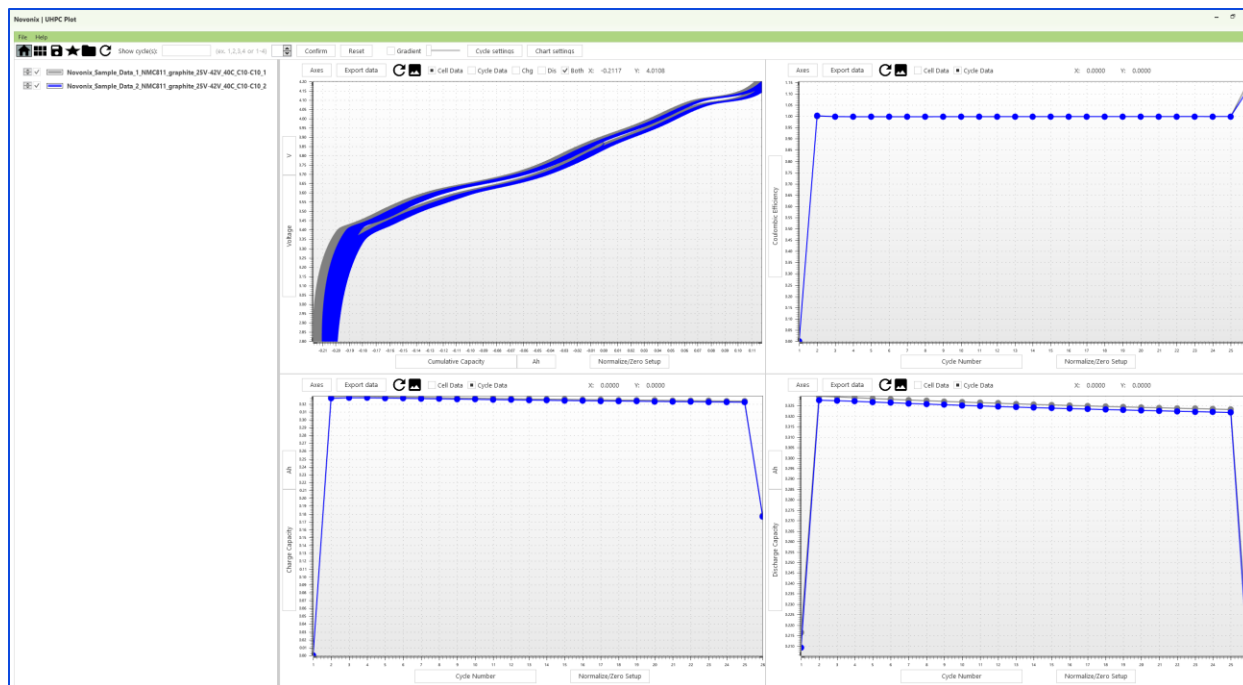


Figure 49: The main UHPC Plot view, showing two data files plotted across four graphs.

In the default configuration, four standard graph panels will be shown, with the data for multiple files shown in different colours overlaid on each panel. The default standard graphs are:

- Voltage vs. Cumulative Capacity,
- Coulombic Efficiency vs. Cycle Number,
- Charge Capacity vs. Cycle Number and
- Discharge Capacity vs. Cycle Number.

7.2 Data File Panel and Graph Settings Bar

7.2.1 Data File Panel



Figure 50: The data file panel's command buttons.

The panel on the left lists the data files loaded. Un-checking a file will remove that file from the graphs. Right clicking and then selecting “Delete File(s)” on a selected file will remove all selected files from the list.

Home screen:

Clicking the “home” button (*Figure 50*, first on right) will return the view from the Multi Panel to the default, four-graph view.

View Files Separately:

Clicking on the “view files separately” button (*Figure 50*, second from right) (or selecting File -> Multi Panel) will allow you to view whatever files are selected individually. Each file will have its own graph, as shown below.

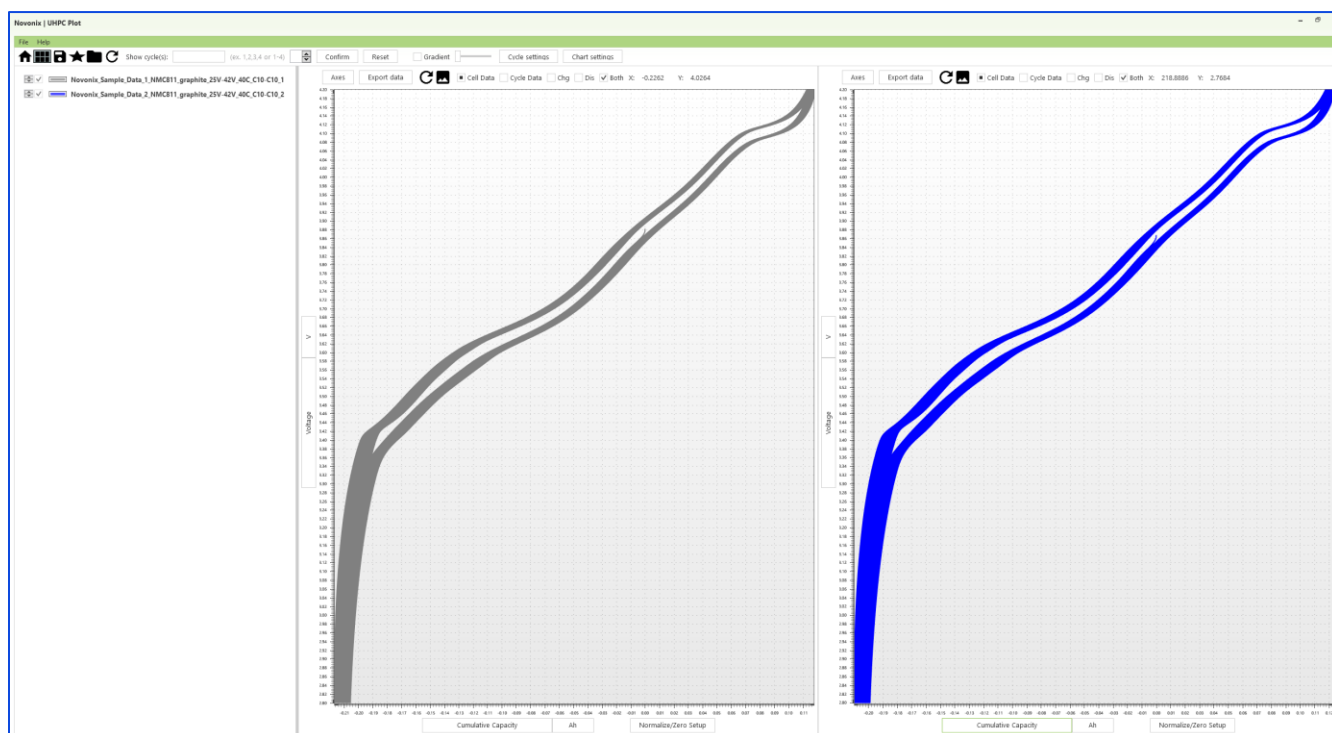


Figure 51: Multi Panel view showing the two loaded files separately.

Save:

Clicking on the “save” button (*Figure 50*, third from the right) (or selecting File -> Save) will bring up a new form, shown below. This form is used to generate ASCII text files that can be used to create presentation quality graphs externally.

☐ Combine output files from different cells

One file per cell will be written containing all of the checked options (CycleSummary)

☐ Separate selected traits (Compares each against time or cycle)

☐ vs Cycle ☐ vs Time ☒ vs Time and Cycle

☒ % Charge capacity ('Qcpercent')
☒ % Charge energy ('Ecppercent')
☒ % Discharge capacity ('QdPercent')
☒ % Discharge energy ('EdPercent')
☒ Average charge voltage ('AvgVc')
☒ Average discharge voltage ('AvgVd')
☒ Charge capacity ('Qc')
☒ Charge slippage ('SlipC')
☒ Charge endpoint ('CendPt')
☒ Charge energy ('Ec')
☒ Coulombic efficiency ('CE')
☒ Coulombic inefficiency ('CIE')
☒ Coulombic inefficiency/hour ('CIEhr')
☒ Delta V ('DeltaV')
☒ Discharge capacity ('Qd')
☒ Discharge slippage ('SlipD')
☒ Discharge endpoint ('DendPt')
☒ Discharge energy ('Ed')
☒ Energy efficiency ('EE')
☒ Fade ('Fade')
☒ Percent charge slippage ('SlipCpercent')
☒ Percent charge endpoint ('CendPtPercent')
☒ Percent discharge slippage ('SlipDpercent')
☒ Percent discharge endpoint ('DendPtPercent')
☒ Zeroed Percent charge endpoint ('ZeroedCendPt')
☒ Zeroed Percent discharge endpoint ('ZeroedDendPt')
☒ Percent capacity fade ('CapacityFadePercent')

One file per cell will be written containing all of the checked options (DetailedVQ)

☐ Cycle ('Cycle #')
☒ Capacity ('Q')
☒ Voltage ('V')
☒ dQ/dV ('dQ/dV')
☒ dV/dQ ('dV/dQ')
☐ RunTimes ('RunTime (Hrs)')

One multi-column file will be written per cell for each of the checked options (DetailedPreset)

☐ Capacity vs Voltage (discharge) for each cycle ("nnnn-Qd_V0.csv")
☐ dQ/dV vs. capacity for each cycle ("nnnn-dQdV_Q-Cycle.csv")
☐ dQ/dV vs. capacity for each cycle, capacity zeroed ("nnnn-dQdV_Q-Cycle_QcZero.csv")
☐ dQ/dV vs. voltage for each cycle ("nnnn-dQdV_V-Cycle.csv")
☐ dV/dQ vs. capacity for each cycle ("nnnn-dVdQ_Q-Cycle.csv")
☐ dV/dQ vs. capacity for each cycle, capacity zeroed ("nnnn-dVdQ_Q-Cycle_QcZero.csv")
☒ Voltage drop during storage vs. time ("nnnn-T_Vdrop.csv")
☐ dQ/dV vs. capacity ("nnnn-dQdV_Q.csv")
☐ dQ/dV vs. voltage ("nnnn-dQdV_V.csv")
☐ dV/dQ vs. capacity ("nnnn-dVdQ_Q.csv")
☐ Voltage vs. capacity ("nnnn-VQ.csv")

Saved data output units: Reference cycle number

Figure 52: The top segment of the save form. Two other panels, unshown, are also part of the save form.

Once you have selected the data files you wish to create, clicking the “Generate Files” button will generate all those files in the location selected. You will be prompted to select a base file name. Each data file generated will contain this name, together with the extension listed in the selected data file type.

Reload default configuration:

To reload the default configuration, click the corresponding button (*Figure 50* above, third from left, star shaped). Clicking on the “reload default configuration” button will load the latest graph panel configuration. This can be changed according to user preference by selecting File -> Save page as default values from the top toolbar. The current graph panel configuration in view will be saved as the default.

Open:

Additional files can be loaded by selecting File -> Open from the top toolbar, or by clicking the “open” button (*Figure 50* above, first on left, folder shaped) and selecting the additional files needed.

Reload:

Selecting File -> Reload from the top toolbar or clicking the “refresh button” (*Figure 50* above, second from left, circular arrow shaped) will reload the data files. This would typically be used to reload files for cells that are currently running on the system where the data is not currently shown in the graph.

7.2.2 Graph Settings Bar




Figure 53: The menu bar above the graph panels.

Show Cycle(s):

Enter in numbers separated by “,” or a range of cycle numbers for example “1-4”. Click on “Confirm” to update the graph display only the cycles specified.

Gradient:

The gradient feature shows a different colour shade for each cycle. The colour is based on the original colour for the cell. Moving the slider bar represents how much of a difference the color will fade from the previous cycle colour. To enable this feature, simply checkmark the gradient checkbox.

Cycle Settings:

This opens the Cycle Settings window shown below. Datafile cycles use the cycles created by the protocol during runtime, calculated cycles use an internal algorithm to determine the correct cycle distribution using the settings found under ‘Calculated Cycle Settings.’ Including the first half cycle is important for managing the first discharge, before a charge/discharge cycle.

How the coulombic efficiency calculations are affected by cycles can also be configured in this window.

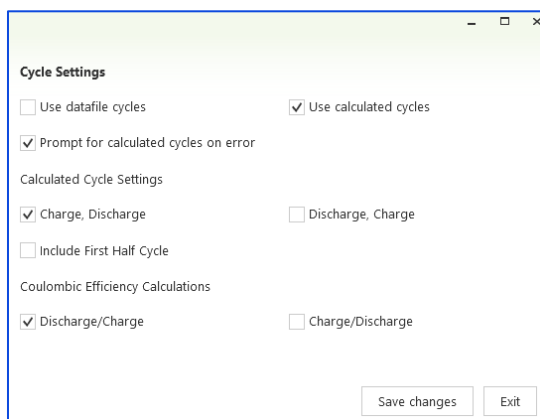


Figure 54: The Cycle Settings configuration window.



Checking this box ensures that the first full cycle for each data file is correctly identified. This is the first complete charge step followed by a discharge step. This is important when a discharge step is used before the first charge step in a protocol, which can lead to erroneous UHPC parameter values.

Chart Settings:

Allows the user to select various chart display options such as line size, symbol size, etc. and toggle the display of legends and axes. “Drag left to reset zoom” can be disabled, causing dragging left on a graph to zoom in, similar to dragging right. *Hover over settings options for tooltips.*

Chart Settings

Chart Line Size

2

Axes Font Size

13

Symbol Size

8

Line Style

Solid

Symbol Shape

Circle

☐ Show Legend

☐ Show Title

☒ Show Grid Lines

☐ Background Chart Gradient

☒ Drag left to reset zoom

☒ Hide Resume datapoint

Show Endpoint Data

Last Endpoint Only

☐ Hide Data HoverOver

☒ Connect Step Endpoints (cell data)

☐ Connect Missing Cycles (cycle data)

☐ Single Graph Only (restart req.)

☐ 4-Graph default on startup

Save changes

Exit

Figure 55: The chart settings menu.

7.3 Graph Panels

There are two styles of graph:



- **Cell data** plots all data points collected (e.g., voltage vs. capacity for multiple cycles).
- **Cycle data** plots a summary point for each cycle collected. You can change the style of a graph by selecting the appropriate choice on the top of each graph.

When plotting cycle data, there are added option boxes to allow the selection of only discharge cycle data, only charge cycle data, or both. You can change the parameters within a given graph style by clicking the “axis label” button and selecting from the list displayed. You can change the scale of the axes by clicking the “Axes” button and inputting the x or y-axis max min values. The export data button allows one to generate an ASCII text file for only the data contained on the current graph panel.

Right clicking and dragging will allow you to freely move around the axis to view data points better. Left click and drag will allow you to draw a zoom in box to zoom in on any specific area. Ctrl left click will allow you to zoom vertically. Shift left click zoom horizontally.



Refresh button will reset the graph to default zoom.



Export as PNG will save the graph in PNG format.

The same list of files loaded on the front screen will be present in the left-hand panel list. The main part of the screen contains four lists of files that could be generated:

Top Left panel:

Cycle based summary data (e.g., Coulombic Efficiency v. Cycle number). This will generate a separate data file for each option selected. The data file will be arranged with Cycle number in the first column and then a separate column of data for each data file present.

Top Right Panel:

Time based summary data (e.g., Coulombic Efficiency v. Run time). This will generate a separate data file for each option selected. The data file will contain two columns for each data file. The first of these two columns will contain run time for each cycle and the second column will contain the summary value for that cycle.

Bottom Left Panel:

Raw data files. This will generate a separate file for each data file selected and for each of the output file types in the list selected.

Bottom Right Panel:

Raw data files. This will generate a single file for each of the output file types in the list selected. Each



file will contain two columns for each data file selected.

Using the plotter:

Keyboard/Mouse Input	Graph Actions
Ctrl + scroll wheel	Scale the plot by the y-axis
Shift + scroll wheel	Scale the plot by the x-axis
Scroll wheel up	Zoom into the graph, focused on the mouse
Scroll wheel down	Zoom out
Click and drag right	Zoom into the area of the displayed box
Click and drag left	Reset zoom to default
Click and drag on an axis	Pan in the x- or y-direction
Double Click on graph	Create Label on graph

7.4 Data File Formatting

The data files produced by UHPC Control and processed in UHPC Plot are .csv files. Avrion does its best to keep a consistent format to prevent custom parsers from requiring updates.

The current format is as follows:

1	[Summary]																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																									
---	-----------	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--

Figure 56: Sample UHPC Data File

Seen above in Figure 56 is the standard UHPC data file with headers at the top, and the beginning of the test results beginning on line 22 in this example. The headers of the data file contain a few lines that often need extra explanation and are typically just used for backend UHPC Plot Processing, please see below for further explanation.

Step Type: The step column is a number that represents the type of step being executed. See Figure 57 for a full list.

```

Open Circuit Storage = 0
Constant Current Charge = 1
Constant Current Discharge = 2
cccvCharge = 3 (This is only used in a protocol file not data file)
cccvDischarge = 4 (This is only used in a protocol file not data file)
Repeat = 5
Increment = 6
cccvChargeCurrent = 7
cccvChargeHold = 8
cccvDischargeCurrent = 9
cccvDischargeHold = 10
Suspended = 14
SetTemperature = 19
EIS = 20

```

Figure 57: Step Type List

Step Position: Step position is used to help differentiate what is happening during a test

- Step Position 0 is used to indicate a regular datapoint in a step.
- Step Position 1 is used to indicate the first datapoint in a step.
- Step Position 2 is used to indicate the final datapoint in a step.
- Step Position 3 is used to indicate the first datapoint that reached end conditions in a step.
- Step Position 4 is used to indicate the step was stopped.
- Step Position 5 is used to indicate the step was suspended.
- Step Position 6 is used to indicate the step was resumed from snapshot (or suspend).

7.5 Configuration Files

The UHPC Plot software can generate and load configuration files (*.JSON files) that can be used to save a specific graph configuration setup and list of data files and load the setup later without needing to set the configuration as a default or redo the graph settings.

By default, when starting the UHPC Plot software, the program can open both data files (*.csv) and configuration (*.JSON) files. Configurations can also be loaded manually through the File -> Load Configuration command from the top toolbar. Similarly, configurations can be saved using the File -> Save Configuration command from the top toolbar.

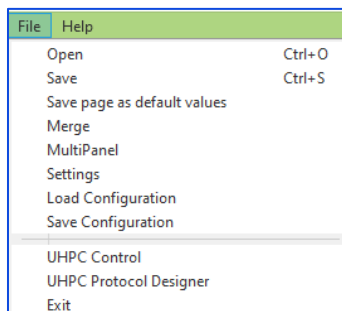


Figure 58: The File drop-down menu showing the Load Configuration and Save Configuration options.

In the event the configuration file is associated with data files that no longer exist or have been moved, the program will alert the user and still load the configuration, but without loading in the data




files that could not be found. If the data files were simply moved, opening them in the software and re-saving the configuration will allow them to be accessed again.

Appendix A – Temperature Control


Using the new Avrion IP-enabled thermal chambers, temperature of the thermal chamber can be controlled during a cell test without any operator intervention. Protocols can be created that specify the temperature set point, and how stable the temperature should be before proceeding to the next step. The following sections will help.

Connecting a Thermal Chamber to UHPC Control


1. Open UHPC Control Software
2. On the top toolbar, click on Settings
3. In the dropdown, click on Startup Configuration
4. Click on Add Thermal Chamber (Green + Icon)
5. This will open a window for the user to configure connected IP-enabled Thermal chambers
6. Assign a Chamber Name that helps you identify it.
7. If the IP Address is pre-populated on the box beside the temperature controller device IP, click on Validate IP to see if the connection is successful.

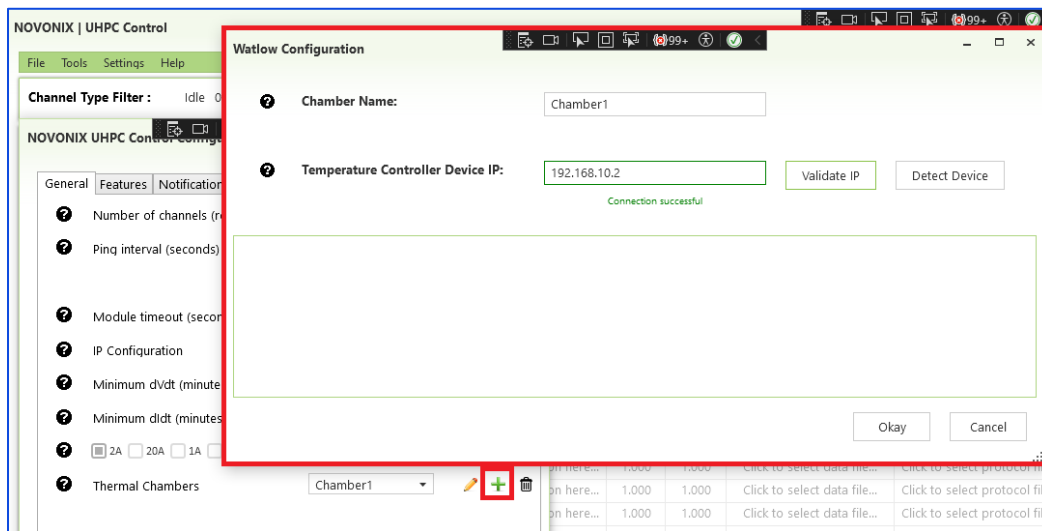

8. If no IP has been pre-populated or connection unsuccessful, click on Detect Device.
9. Follow the Steps mentioned on the dialog box below in the software to find the Serial number of the Watlow Device.

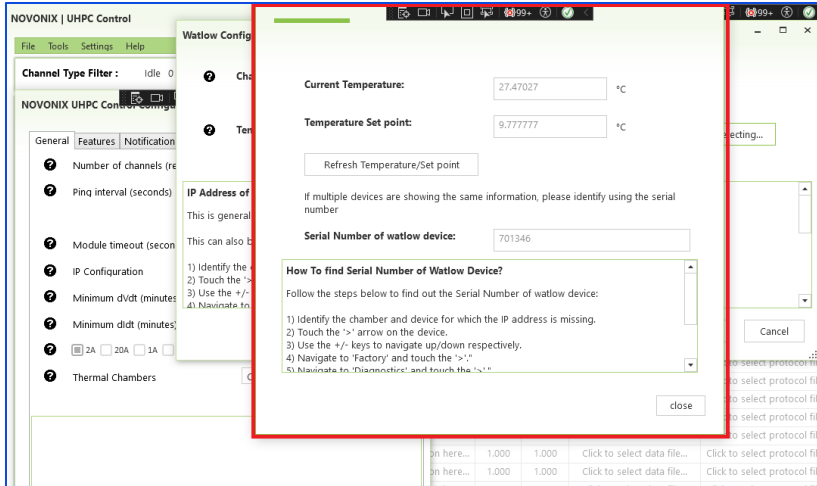

10. After successfully adding the thermal chamber, you can assign an individual thermal chamber to an individual channel.
11. Save the Startup Configuration and return to the main UHPC Control interface.
12. From the main UHPC Control channel grid, right click on the channel(s) you wish to have associated with the chamber, and then click on Assign Chamber to select the chamber name that has been set previously.

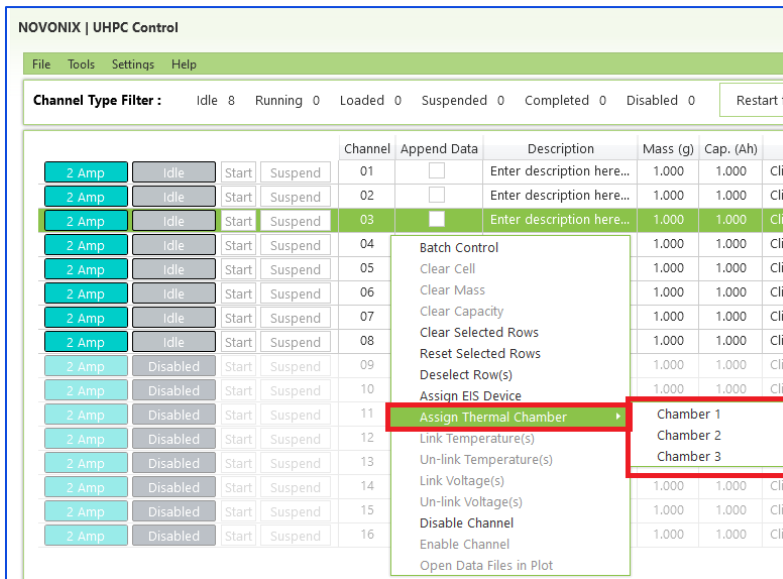

13. The first time a chamber is assigned to a system, the user will be prompted, if they wish to display the Connected Chamber Name and Chamber Temperature columns.

Would you like to show the Chamber Name and Chamber Temperature columns in the channel grid?

yes no

14. If “no” was clicked... In the future, if the user wishes to display the thermal chamber associated with a channel display grid, click on settings from the top toolbar.
15. Click on Column Configuration.
16. Ensure the checkbox next to Connected Chamber Name and Chamber Temperature is set to true.

Reset


☒	Cap. (Ah)	Capacity
☐	Area (cm2)	Area
☒	Data File Name	Data File Name
☒	Protocol File Name	Protocol File Name
☒	Temp	Temperature
☒	Run Time	Run Time
☒	Step Time	Step Time
☒	Current	Current
☐	Resistor	Resistor
☒	Potential	Potential
☒	Step Capacity	Step Capacity
☐	Cumulative Capacity	Cumulative Capacity
☒	Cycle Num	Cycle Num
☒	Active Step Display	Active Step Display
☒	Chamber Name	Connected chamber Name
☒	Chamber Temp	Chamber Temperature
☒	EIS Device	Linked EIS Device
☒	Channel Notes	Channel Notes

ok cancel



Setting Temperature with UHPC Protocol

On the protocol step control list, there is a new step type called Set Temperature.

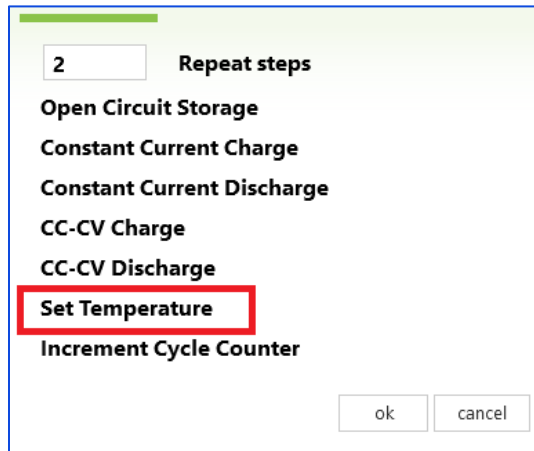


Set Temperature Step Type:

A Set Temperature step control type allows for temperature control of Avrion IP-Enabled thermal chambers. When the set temperature step starts, a command will be sent to the thermal chamber temperature controller associated with the running channel. The temperature will be set once, and then run until the end step conditions are met. The command will be sent again if the step is suspended and resumed. Step control conditions work as with all other protocol steps, but with two additional end step conditions, Temperature Variance and Temperature Hold.


By default, for Set Temperature; Temperature Variance and Temperature Hold control conditions are used together with an AND condition modifier. Which causes the Set Temperature step to end successfully when the temperature is held at the set point within the variance tolerance for the total hold time. Temperature Variance and Temperature Hold both use chamber temperature, rather than cell temperature when measuring variance.

Note: While it may be tempting to use a super tight temperature variance setting like 0.5C, in testing, a hold of about 1C of variance has worked best across the supported temperature ranges.

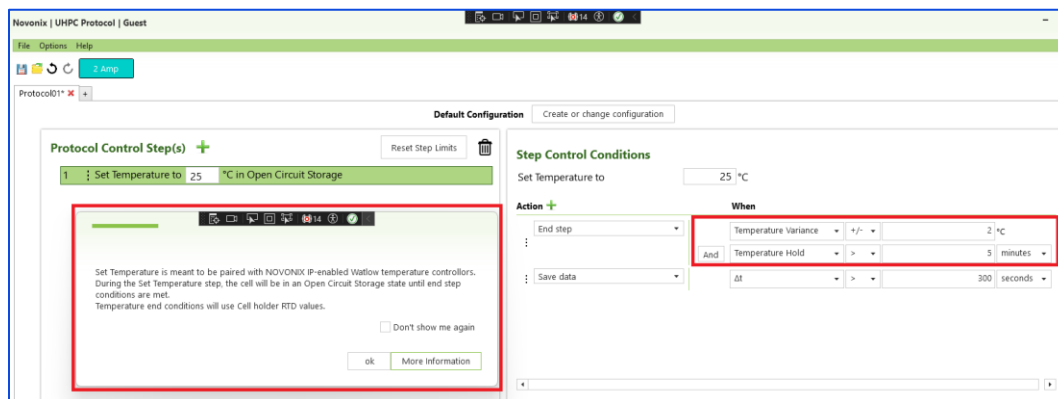

Temperature Control with Multiple Channels

As of UHPC Control version 2.13.0, temperature control for multiple channels has been simplified, and synchronization is controlled with a system setting enabled by default labelled *Sync Thermal Chamber Channels*.

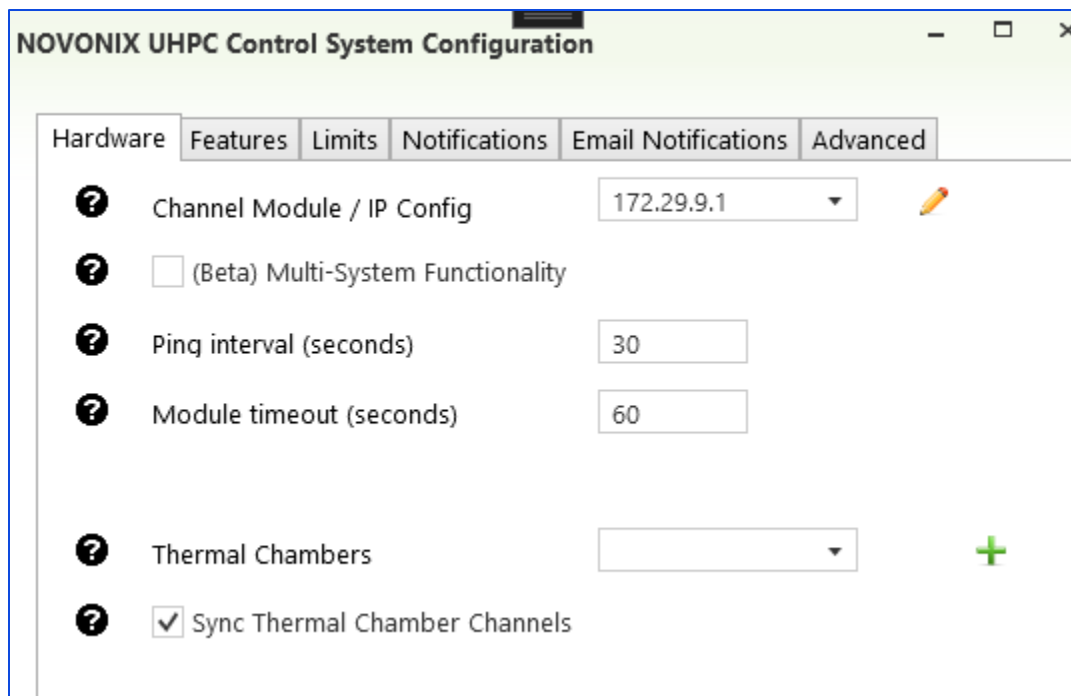

When enabled, all channels connected to an IP-Enabled thermal chamber will wait at the 'Set Temperature' step without executing the temperature change until all running channels assigned to the same thermal chamber are also at the set temperature step.

If channels are out of sync and different temperature set points are being used simultaneously, UHPC will choose the majority, and halt the running protocol for the other channels out of sync. Step numbers do not need to match, just the temperature set points.

Warning: Assigning different protocols to the same thermal chamber is allowed (with warning popup), but if one protocol has no set temperature step for example, all other channels on the same thermal chamber could be disrupted from set temperature executing properly. In cases like these, where a user wants most channels to stay synchronized in a chamber, and others can run freely, consider unassigning the assigned thermal chamber from the channel configuration. This can be accomplished by right clicking the channel and clicking Unassign Thermal Chamber.

Temperature Linking

While not required for thermal chamber / protocol temperature control, Temperatures can be linked between channels. So that all selected channels have a temperature that matches one another based off one "anchor" channel. This may be useful to some users, under special conditions.

This can be accomplished by selecting two or more channels, then right-clicking and selecting Link Temperature(s).

Protocol File Name	Temp
Batch Control	33.001°C
Clear Cell	43.001°C
Clear Selected Rows	53.001°C
Reset Selected Rows	63.001°C
Deselect Row(s)	---
Link Temperature(s)	---
Un-link Temperature(s)	---
Link Voltage(s)	---
Un-link Voltage(s)	---

Figure: The right-click menu showing the Link Temperature(s) option.

The anchor is the channel that copies its temperature to the other channels. The color display will indicate which channel is the anchor.

Which channel would you like to be the anchor?

Select the color to represent the link

Figure: The temperature assignment menu.

Temp
32.999°C
32.999°C
32.999°C
32.999°C

Figure: Linked temperatures as assigned by the previous box. The anchor channel is the topmost channel.

Appendix B – Gamry EIS Integration

Using Gamry EIS modules connected via USB to the UHPC PC, Electrochemical Impedance Spectroscopy (EIS) testing can be conducted at any point during a cell test without any operator intervention. Protocols can be created that specify the EIS test conditions. The following sections will help:

First Time Gamry Hardware Setup

First get started by registering your new Gamry device online at <https://www.gamry.com/client-portal/my-account/>. This will allow you to download the Gamry software onto your Windows PC.

Once the Gamry unit has been placed into the rack with the UHPC hardware, the next step is to plug in the cables.

Begin by plugging in the USB cable and Gamry supplied power cable in the rear of the unit. Please note that Gamry Ethernet connection is not currently supported by UHPC Control.

Next begin connecting the Gamry cell cable to the front of the Gamry unit. Below you'll find two common examples and cable types.



Figure 59: Gamry Interface 1000 front panel with cell cable attached



Figure 60: Gamry EIS Box front panel with cell cable attached

The EIS Box variants have many more cables than the standard Gamry Interface unit, each column of two line up to a single UHPC Channel.

For each column on the front panel of the EIS Box, plug in the matching Current Connection cable to the top panel, and the Sense Connection to the bottom panel.

Tip: To prevent mixing cables once everything has been plugged in, we often label each end of each pair of Gamry cables with a simple ID, so that the Current Connection and Sense Connection remain paired up.

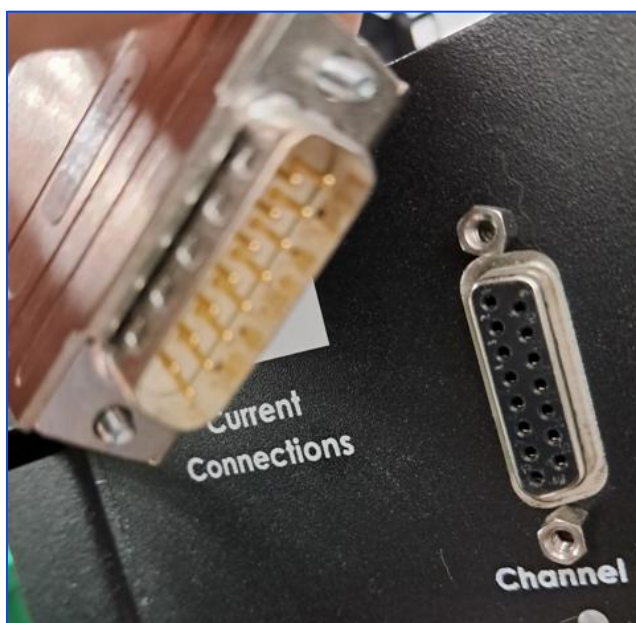


Figure 61: Gamry EIS Box Current Connection Cable

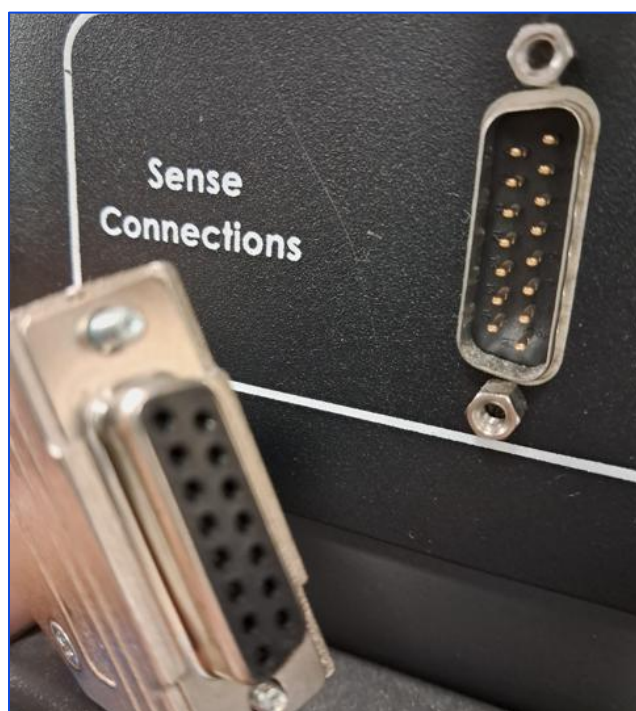


Figure 62: Gamry EIS Box Sense Connection Cable

Once the Single Cell Cable, or paired Sense Connection and Current Connection cables have been plugged into the Gamry unit, the other ends of the Gamry cables plug into the UHPC Gamry Interconnect Split Cable seen below in Figure 63: UHPC 2A/10A interconnect cable with Gamry connectors. The specific variant depends on which Gamry unit you've purchased, and our Sales or Support team can help determine which cable is required.

These cables are color coded to match the Gamry cables. Simply match up the colours of Gamry connectors with the matching coloured UHPC Interconnect connectors as seen in the Figure 64: Gamry Connectors plugged into UHPC Channel Cable below. Repeat for all EIS channels.

Note: The coloured connectors that join the UHPC cables to the Gamry cables should be attached at the end of the UHPC interconnect cable that plugs into the UHPC Thermal Chamber. The opposite end of the UHPC interconnect cable, which does not have any EIS connections, plugs into the UHPC Channel Module. See the figure for clarification.



Figure 63: UHPC 2A/10A interconnect cable with Gamry connectors



Figure 64: Gamry Connectors plugged into UHPC Channel Cable

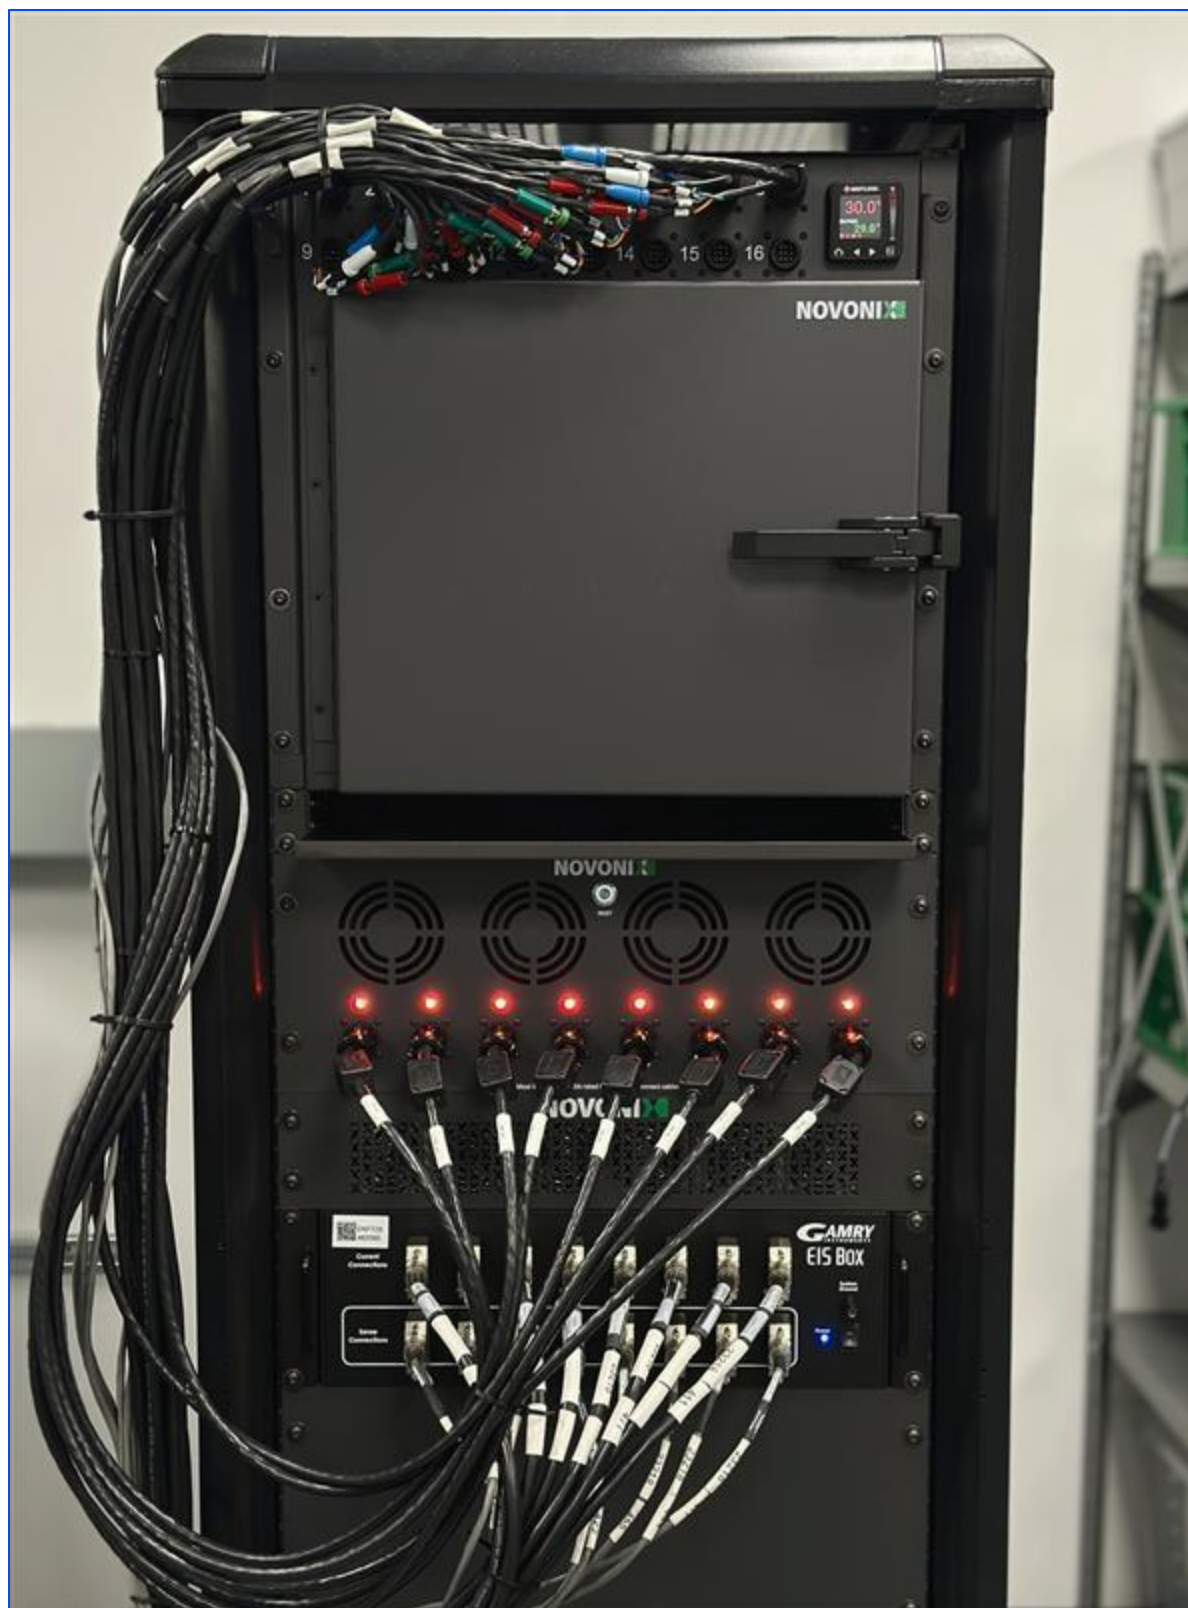


Figure 65: Complete Integrated UHPC-Gamry Setup

Connecting Gamry Hardware to PC and Updating Gamry Firmware

After connecting a Gamry EIS device via USB to the UHPC computer, if UHPC cannot detect the device some troubleshooting may be required. Typically, this issue is resolved by unplugging the Gamry USB cable and/or powering the Gamry device off and back on.

If this is the **first time** using the Gamry device with UHPC Control, the Gamry device could need its firmware updated. Please follow the steps below on updating the Gamry firmware version.

Install and launch Gamry Instruments Framework, which should be provided along with your Gamry device, or via the internet, and on the top toolbar click Options -> Instrument Manager.

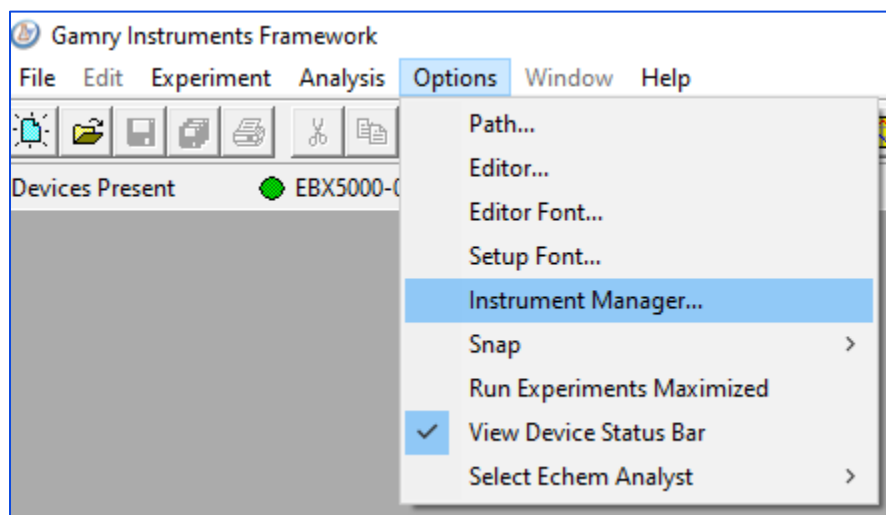


Figure 66: Gamry Instruments Framework

Find the Gamry device on the Instrument Manager device list and run the update. Once the firmware is updated to the latest version, and four green checkmarks appear under the device status, close the Gamry Instruments Framework and try connecting via UHPC Control again.

If the Gamry device cannot be detected by Gamry Instruments Framework or the Instruments Manager, then please [contact Gamry](#) for assistance.

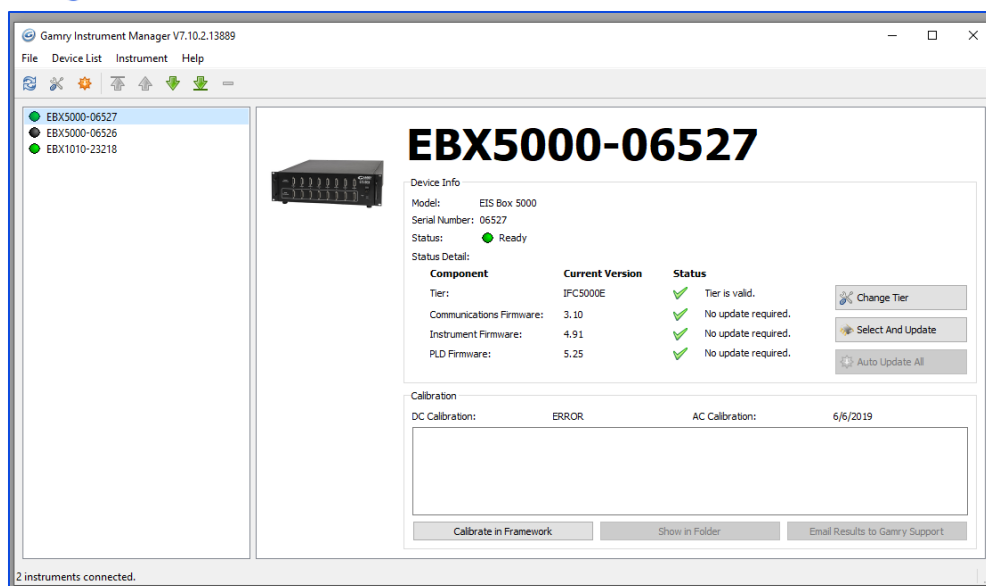


Figure 67: Gamry Instruments Manager Update Successful

Connecting an EIS Device to UHPC Control

Ensure that the Gamry device is connected to the UHPC computer via USB. With UHPC Control launched, right click a channel to assign the EIS device to and click “Assign EIS Device”.


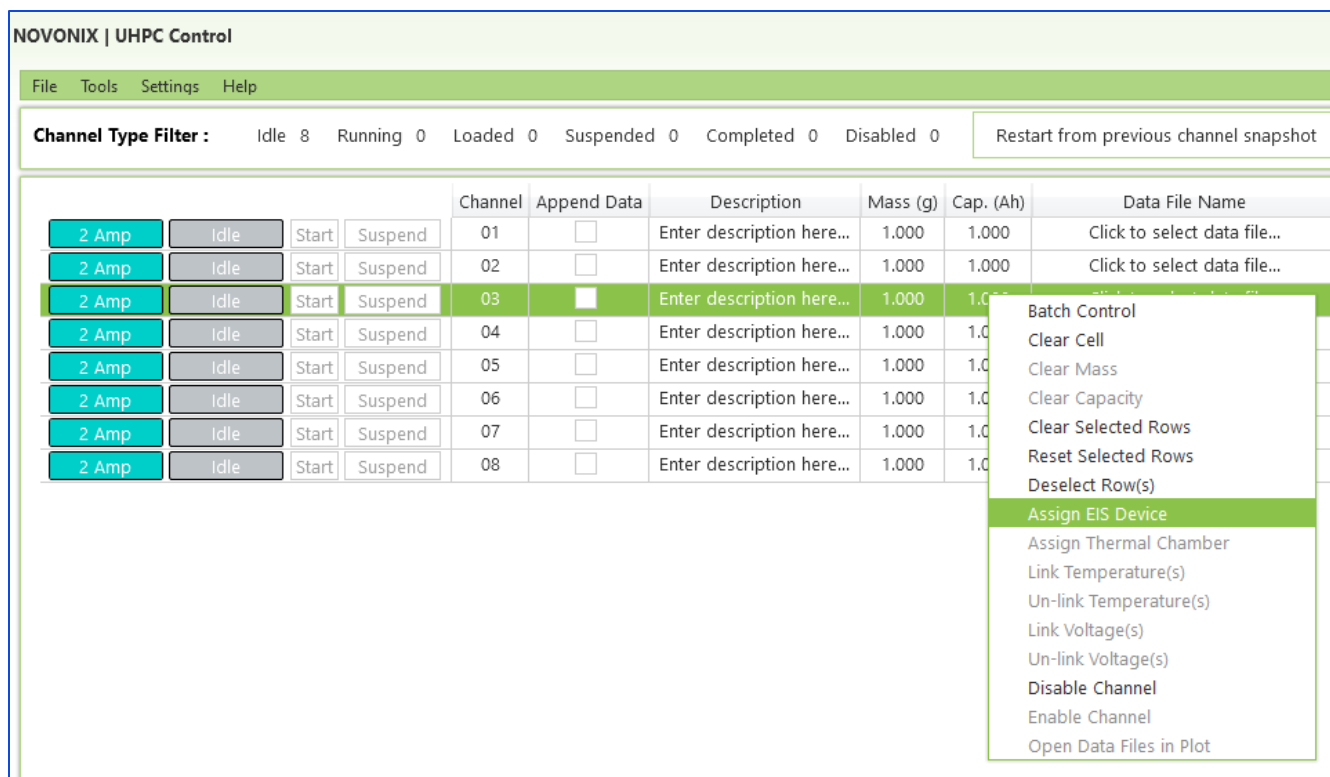


Figure 68: Assign EIS Device

After clicking “Assign EIS Device” a configuration window will appear, allowing the operator to select UHPC Channel, Gamry Device, and the corresponding EIS channel.

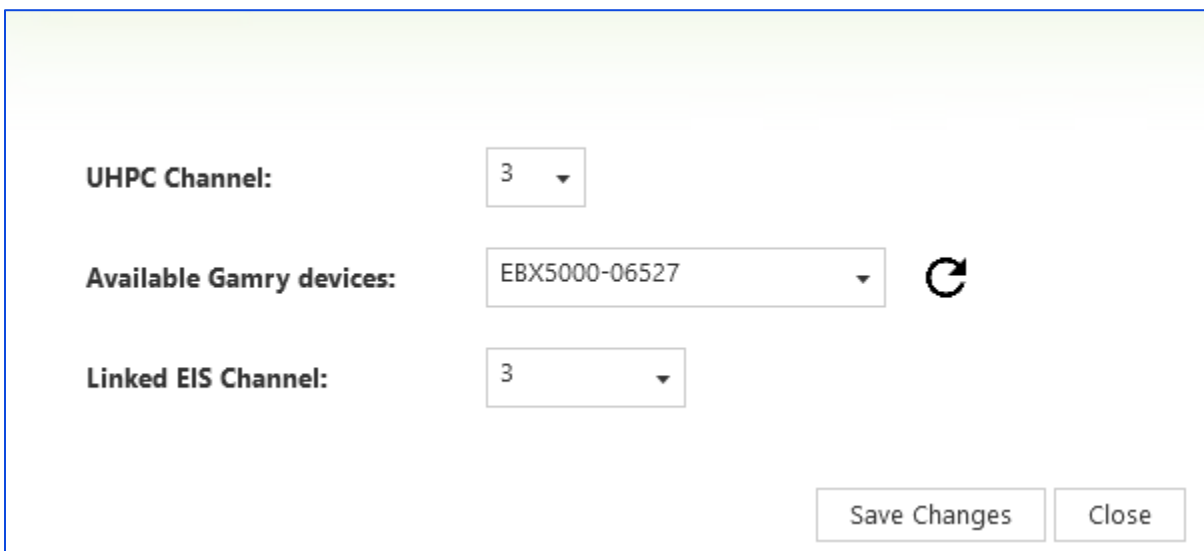

The image shows a configuration window titled "EIS Channel Configuration". It contains three main sections:

- UHPC Channel:** A dropdown menu with the value "3" selected.
- Available Gamry devices:** A dropdown menu showing "EBX5000-06527". To the right of this dropdown is a circular refresh icon.
- Linked EIS Channel:** A dropdown menu with the value "3" selected.

 At the bottom right of the window are two buttons: "Save Changes" and "Close".

Figure 69: EIS Channel Configuration

UHPC Channel: The UHPC channel to assign an EIS device to.

Available Gamry Devices: List of all connected Gamry EIS devices. Click refresh to repopulate the list. If the connected Gamry device is not appearing in this list, please see the following section: [Connecting Gamry Hardware and Updating Gamry Firmware](#)

Linked EIS Channel: Many EIS devices are one channel only in which case this value will always default to 1, but some devices may contain additional channels to connect multiple cells to the EIS device at any given time. This value will identify which Gamry EIS channel is connected to the associated UHPC channel. If the list is incorrectly showing 1 channel for a multi-channel EIS device, please contact Avrion for assistance updating the product support.

Multiple UHPC channels can be configured for Gamry at the same time, but if the same Gamry device and channel is selected as an existing channel, the previous channel data will be erased.


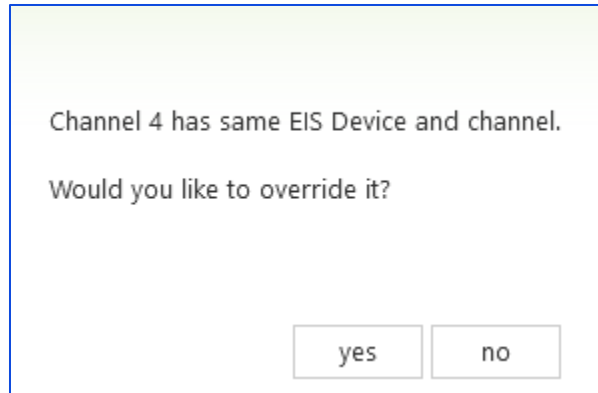


Figure 70: Overwrite EIS Device Warning

IMX8 Multiplexer

Some 1-Channel Gamry EIS devices, such as the Interface 1000/1010 or Reference 600+/620, may be paired with a Gamry IMX8 Multiplexer. This expands a 1-channel EIS system to 8 channels, allowing 8 channels of UHPC Control to pair with EIS on a single device, similar to a EISBOX1010/5000.

Seen below, Configuration for an IMX8 will appear when an IMX8 device has been detected on the Assign EIS Device page. An IMX8 may only be paired with a single Gamry device at a time. Removing a pairing or changing the paired IMX8 device will impact every channel that uses the paired Gamry device.

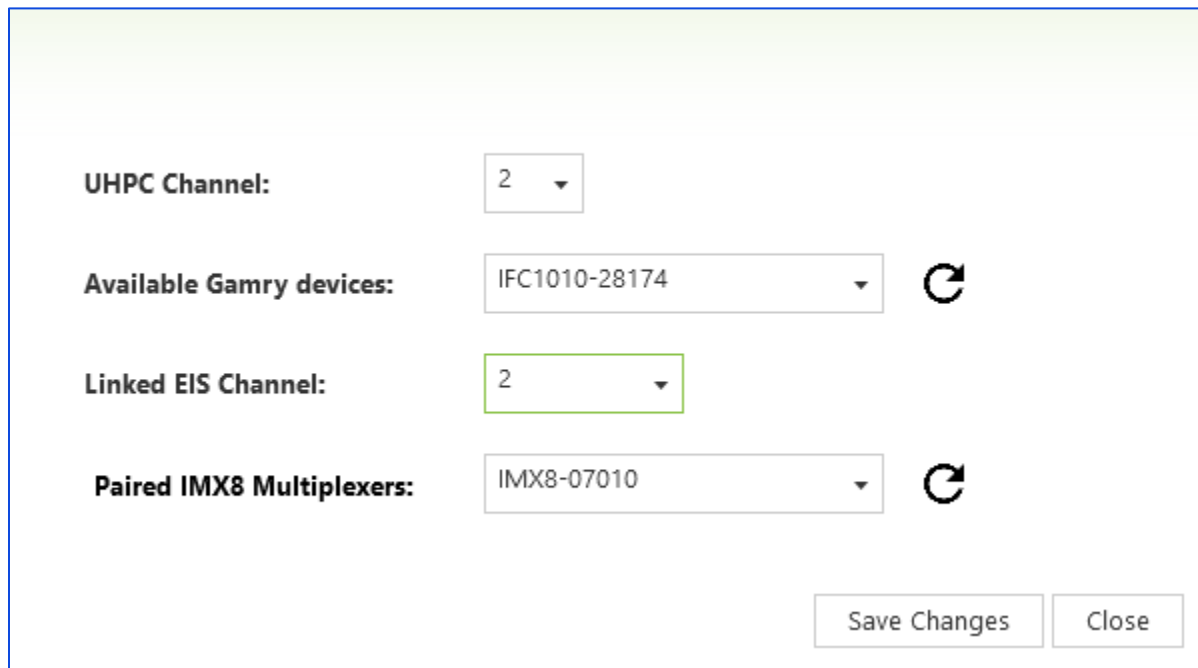

UHPC Channel:

Available Gamry devices: 

Linked EIS Channel:

Paired IMX8 Multiplexers: 

[Save Changes] [Close]

Figure 71: IMX8 Pairing Selection on Assign EIS Device tab

Viewing EIS Channel Information

Once the channel has had a Gamry device assigned, the assigned EIS device can be viewed by updating the Column Configuration.

To edit the Column Configuration: On the top toolbar of UHPC Control, click Settings -> Column Configuration. In the popup window, scroll to the bottom and ensure that “Linked EIS Device” is clicked, and press OK, as shown below in Figure 72: Updating Column Configuration.

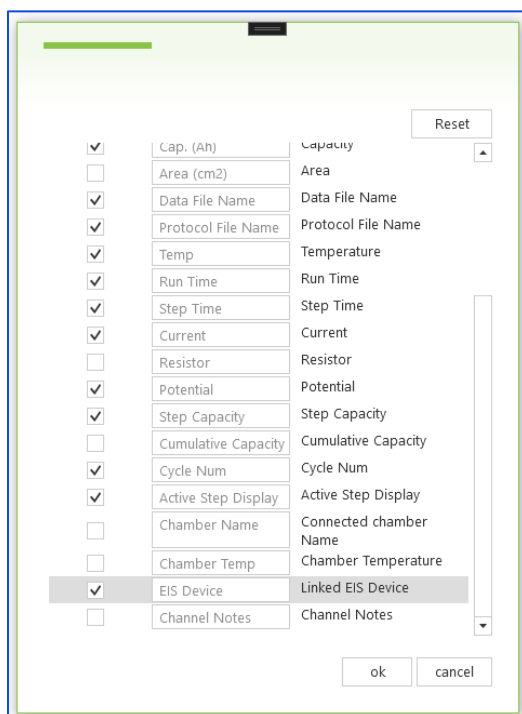


Figure 72: Updating Column Configuration

Once updated, you should see the EIS device, and associated EIS channel # under the EIS Device column in UHPC Control, as shown below in Figure 73: Assigned EIS Device Channel Information.

NOVONIX UHPC Control									
File Tools Settings Help									
Channel Type Filter :				Idle 4	Running 4	Loaded 4	Suspended 0	Completed 0	Disabled 0
				Restart from previous channel snapshot				System name: Sys1	
				Channel	Data File Name	Protocol File Name	Active Step Display	EIS Device	
2 Amp	Idle	Start	Suspend	01	Click to select data file...	Click to select protocol file...	---	EIS CH#: 1, ID: EBS5000-06527	
2 Amp	Idle	Start	Suspend	02	Click to select data file...	Click to select protocol file...	---	EIS CH#: 2, ID: EBS5000-06527	
2 Amp	Idle	Start	Suspend	03	Click to select data file...	Click to select protocol file...	---	EIS CH#: 3, ID: EBS5000-06527	
2 Amp	Idle	Start	Suspend	04	Click to select data file...	Click to select protocol file...	---	EIS CH#: 4, ID: EBS5000-06527	
2 Amp	O	Stop	Suspend	05	2024-08-01_EIS_Test_Run2_CH05.csv	EIS_Test.pro2	EIS step in Queue(2)	EIS CH#: 1, ID: EBS1010-23218	
2 Amp	O	Stop	Suspend	06	2024-08-01_EIS_Test_Run2_CH06.csv	EIS_Test.pro2	Open Circuit Storage	EIS CH#: 2, ID: EBS1010-23218	
2 Amp	O	Stop	Suspend	07	2024-08-01_EIS_Test_Run2_CH07.csv	EIS_Test.pro2	EIS (Freq: 3.162278 Hz)	EIS CH#: 3, ID: EBS1010-23218	
2 Amp	O	Stop	Suspend	08	2024-08-01_EIS_Test_Run2_CH08.csv	EIS_Test.pro2	EIS step in Queue(1)	EIS CH#: 4, ID: EBS1010-23218	

Figure 73: Assigned EIS Device Channel Information

Creating EIS test with UHPC Protocol

On UHPC Protocol there is a new step type called “EIS”.

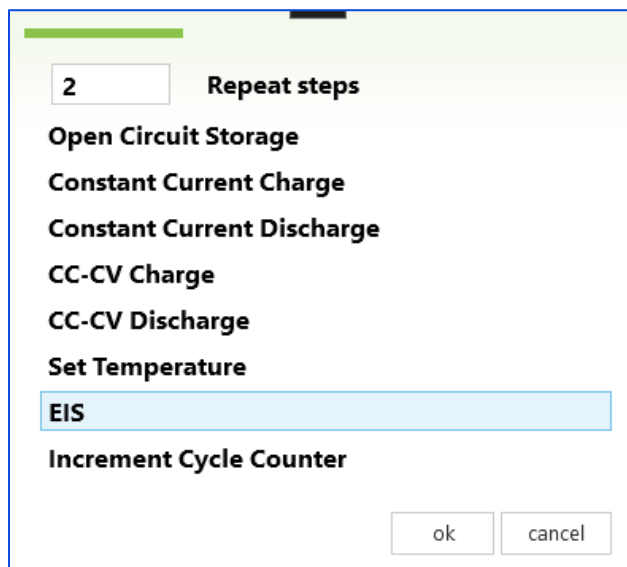


Figure 74: Select Step Type EIS

There are three types of EIS tests that can be run: Galvanostatic, Potentiostatic, and Hybrid.

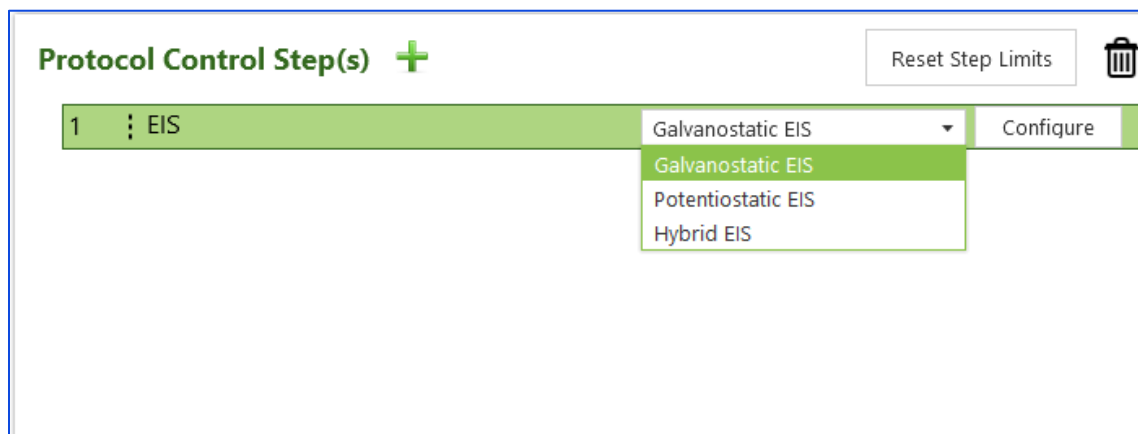


Figure 75: Select EIS Type

Potentiostatic: The most used EIS test, Potentiostatic mode is used when maintaining a constant voltage is crucial. This mode is ideal for studying the electrode processes and battery cell behavior at a fixed potential, making it useful for analyzing the stability and efficiency of the cell under a specific voltage. Researchers often employ this mode to understand the reaction kinetics and to identify the resistive and capacitive elements within the cell.



You wouldn't want to run a test in Potentiostatic mode if the impedance of the cell is very high (small cell), as this could result in unstable voltage control and inaccurate measurements.

Galvanostatic: Galvanostatic mode is employed when a constant current is required during EIS testing. This mode is particularly useful for examining the response of a battery cell to steady current flow, which is representative of real-world operating conditions. It allows for the study of charge transfer resistance and mass transport processes, making it valuable for understanding the performance and limitations of the battery under consistent load.

Avoid using galvanostatic mode if the cell has very low impedance (large cell), as maintaining a constant current can lead to excessively high or low voltages that may damage the cell or distort the data.

Hybrid: Hybrid mode combines the features of both Potentiostatic and Galvanostatic modes, allowing for more versatile and comprehensive EIS testing. This mode can adapt to changing conditions by switching between maintaining a constant voltage or current as needed. It is beneficial for dynamic studies where the battery cell's behavior under varying loads and potentials needs to be analyzed, providing a more complete understanding of the cell's electrochemical characteristics.

Hybrid mode may not be ideal if the system's response is highly non-linear, as the switching between voltage and current control could introduce artifacts or complicate the interpretation of the impedance data.

Each type of EIS can be configured from the default values using the “Configure” button. Each configure page is similar to the Gamry Instruments Framework configuration for the corresponding EIS type.

Running an invalid Gamry EIS protocol may impact testing, at this time UHPC may not validate an EIS protocol to the same extent as Gamry Instruments Framework. When setting up a configuration for the first time, we recommend testing the configuration with Gamry Instruments Framework to ensure that the settings are valid and that the EIS test completes successfully. Improper settings may result in test failures.

It may be valuable to obtain a full impedance spectrum of a cell via the Gamry Instruments Framework before running an integrated UHPC and EIS test. This will help estimate impedance values and confirm the EIS data collected via UHPC Control.

Seen in Figure 76: Impedance Estimations below, are estimations for the impedance of various sized cells, to be used when creating an EIS experiment, this can be done as an alternative to using the EIS device to first run an impedance sweep on an individual cell. In our experience, impedance doesn't need to be exact, but it should at least be in the correct order of magnitude.

Cell	Capacity (Ah)	Z (Ω)
21700	5	0.02
18650	3	0.04
Stacked Pouch	1	0.1
Wound Pouch	0.2	0.5
Coin	0.005	20


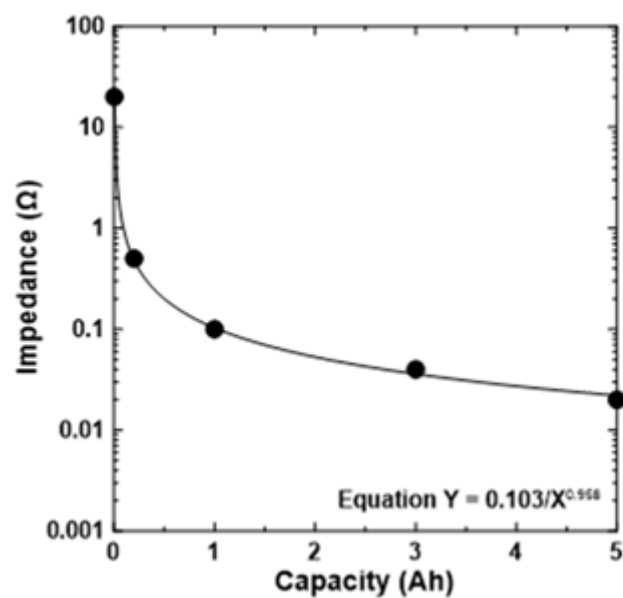


Figure 76: Impedance Estimations

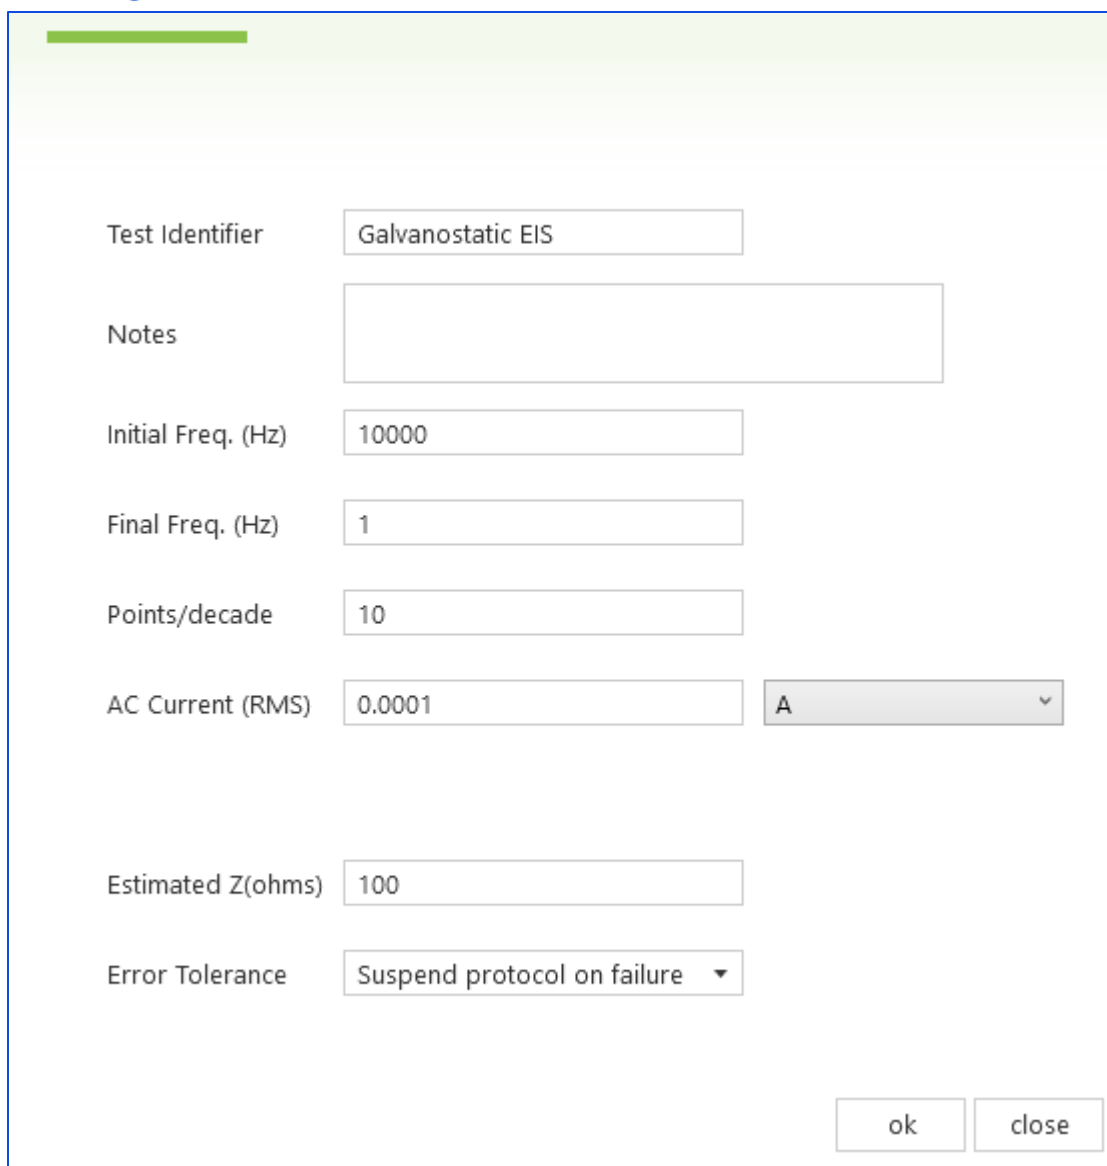

The image shows a software window titled "Galvanostatic Configuration Window". It contains several input fields and a dropdown menu for configuring an EIS test. The fields are arranged in a vertical list, each with a label on the left and an input area on the right. The input areas are text boxes, except for the "AC Current (RMS)" which has a unit dropdown menu. At the bottom right, there are two buttons labeled "ok" and "close".

Test Identifier	Galvanostatic EIS
Notes	
Initial Freq. (Hz)	10000
Final Freq. (Hz)	1
Points/decade	10
AC Current (RMS)	0.0001 A
Estimated Z(ohms)	100
Error Tolerance	Suspend protocol on failure

Figure 77: Galvanostatic Configuration Window

The end conditions and data save conditions for EIS are optional. Channel information values may be recorded by UHPC while running EIS on a cell, but current will always be recorded as 0A. The current sense is disabled for the length of an EIS test for safety reasons, but voltage can be recorded.

Ending an EIS step too early with end conditions may result in an incomplete EIS test file. If using a multi-channel EIS device, concurrent EIS tests may be queued for some Gamry device types, so in some cases, an EIS step may take longer than expected.

Initial Frequency has been set to 10,000hz by default by UHPC Protocol, looking below at Figure 78: Nyquist plot of the impedance spectra 10,000hz , it shows that for most users, the desirable data occurs below even 1000hz. For testing above 10,000hz initial frequency, test conditions will need to be stricter to ensure that the frequency points aren't skipped.

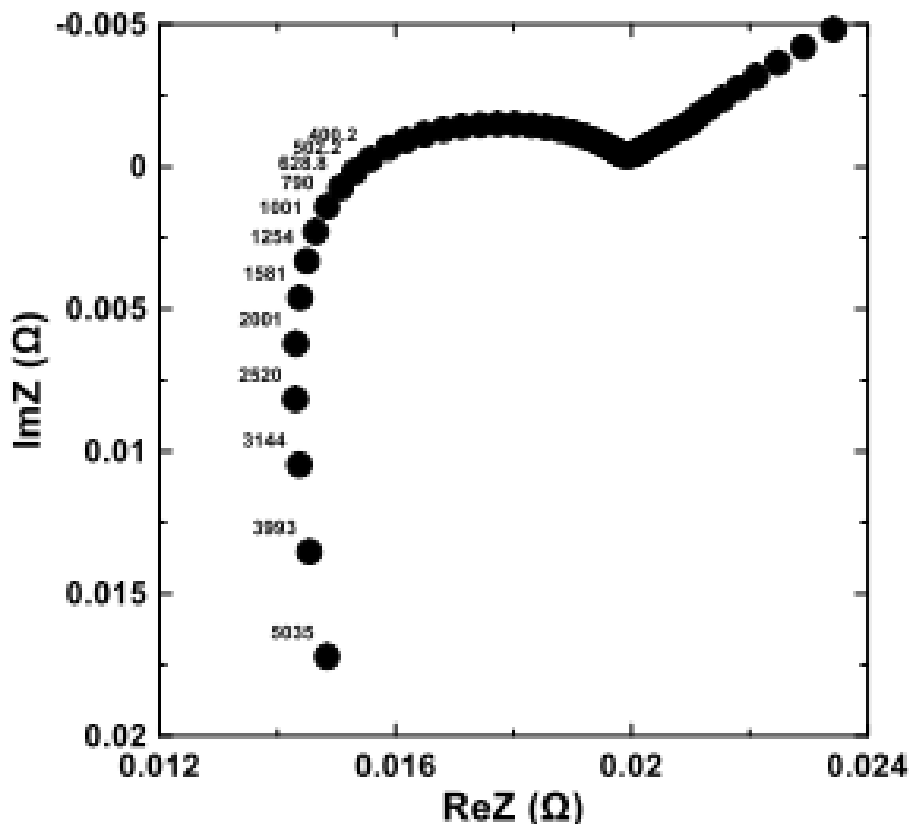


Figure 78: Nyquist plot of the impedance spectra 10,000hz

Running EIS Test with UHPC Control

After assigning an EIS device to a UHPC channel, and creating a protocol containing EIS in UHPC Protocol, all that's required to run a cell test with EIS is starting the test like any other protocol. Simply start the test and wait for it to execute.

Referring to Figure 73: Assigned EIS Device Channel Information, you can see three steps are in EIS, all on the same EIS device. Only one EIS test can execute at a time per EIS device, because Gamry EIS multi-channel devices are multiplexed. This results in the occasional "EIS Step in Queue" Active Step Display.

Validation occurs while assigning a protocol, so an error will be thrown if no EIS device has been detected when assigning a protocol containing EIS as seen in Figure 79: Missing EIS Device Error Window. Similarly, if the assigned EIS device cannot communicate with UHPC, an error will appear in the "Error Log" at the bottom of the UHPC Control screen, as seen in Figure 80: Cannot Communicate with EIS Error Log. If connection with the Gamry EIS device is lost before/during a test, and the system will attempt to reconnect in the background. The UHPC test will not be impacted until the EIS step is reached. The test will halt in error if the EIS device cannot communicate while executing the EIS step.

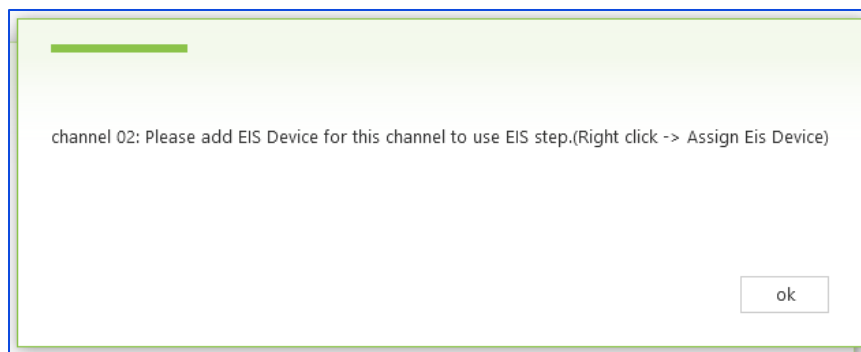


Figure 79: Missing EIS Device Error Window

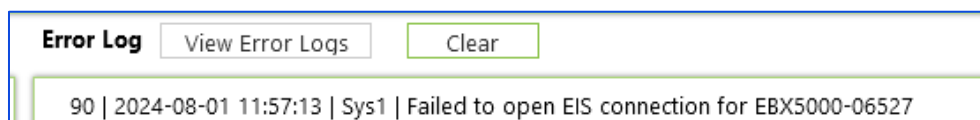


Figure 80: Cannot Communicate with EIS Error Log

Safety Warnings

Do not use Gamry Instruments Framework to run an EIS test or any diagnostics while conducting a test with UHPC Control on the same integrated UHPC/Gamry channel cable, this could result in damage to the UHPC or Gamry hardware. As a safety precaution, if the Gamry unit is connected properly with UHPC Control running, the software will prevent that Gamry unit from being used by Gamry Instruments Framework.

For safety guidelines specific to Gamry devices, please refer to the Operator's Manual provided with your Gamry equipment.

Current ranges on UHPC hardware and Gamry hardware may vary, and EIS tests designed for large cells may contain currents that are damaging to small cells. Always double check that the cell matches the protocol and consider the expected current or voltage response before running a test.

Viewing EIS Data

After running an EIS test, the EIS data will be saved to a folder located with the UHPC test data. The folder name will be labelled "datafileName_EIS". Inside of the folder, each EIS test ran for that test will be labelled "datafilename_step-##_cycle-##_dta". These files will be used like any other Gamry .dta file, using Gamry Echem Analyst, or opened by Gamry Instruments Framework->Analysis->Start Analysis.

Please see Figure 81: View EIS DataWhy EIS Testing with UHPC. below for an example of viewing EIS data in Gamry Echem Analyst. At this time UHPC Plot does not open Gamry EIS .dta data files.

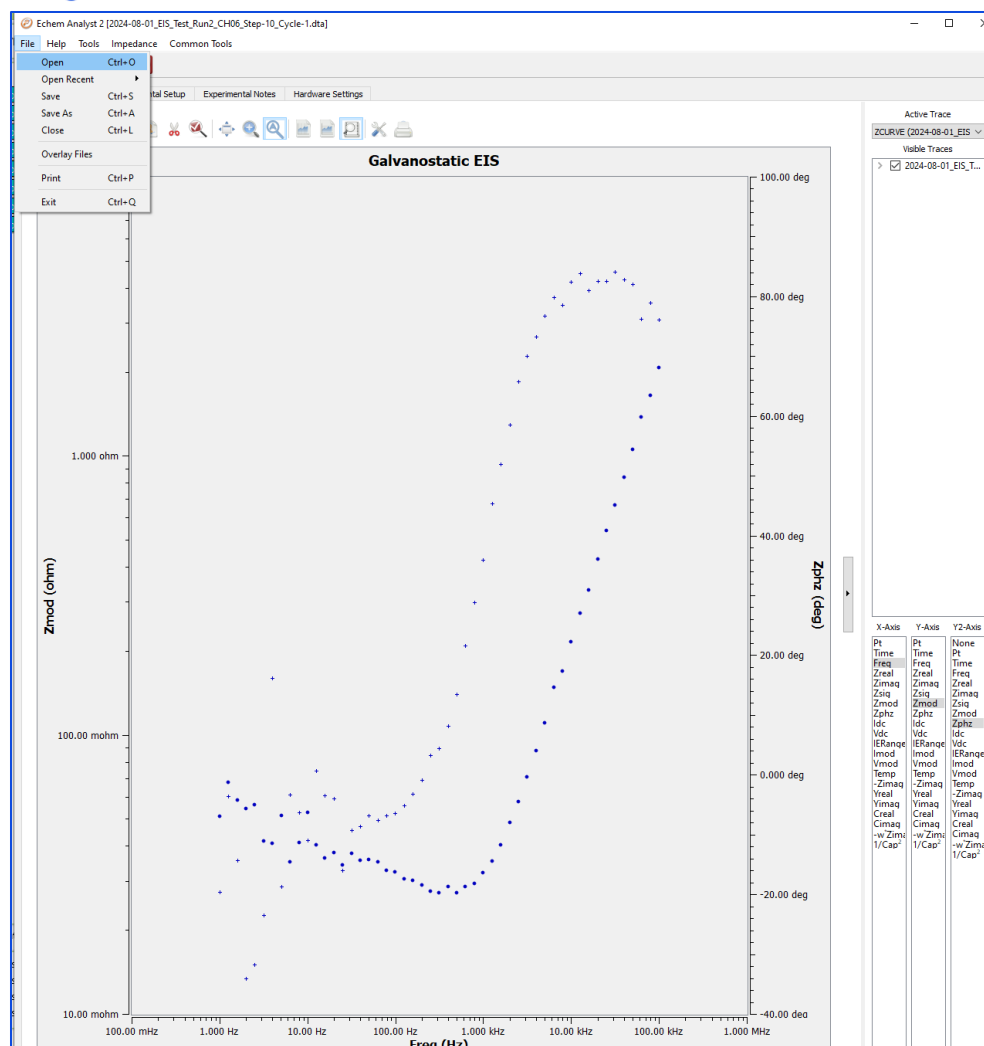


Figure 81: View EIS DataWhy EIS Testing with UHPC

Electrochemical impedance spectroscopy (EIS) delivers results that are complementary to conventional cycle testing. Specifically, EIS measurements reveal kinetic information about individual parts and processes within a cell. When combined with UHPC experiments, a full suite of parameters such as the coulombic efficiency, charge endpoint capacity slippage, and resistances associated with electronic contact, ionic charge transfer and diffusion can be obtained, used to develop a deep understanding cell performance and iterate rapid improvements.

The pairing of a Gamry EIS device with an Avrion UHPC system also eliminates challenges often associated with combined cycling and EIS experiments. These include the labor required to conduct testing on separate machines, managing different temperatures for EIS and cycling experiments, and the complexity of acquiring EIS data at multiple states-of-charge

Appendix C – API Remote UHPC Control Interface

When API Communications is enabled in UHPC Control, a local socket server runs, listening for connections on a user-configured IP address and port. The server accepts valid messages to



command UHPC Control to start, stop, suspend, resume tests, update details, and fetch channel status.

The following sections outline message formats, various commands, and examples.

API Configuration

In the UHPC Control toolbar, navigate to **Settings > System Configuration > Features** to find the 'Enable API Communications' option. Checking this box will start a socket server using the IP and port set in the API Configurations page.

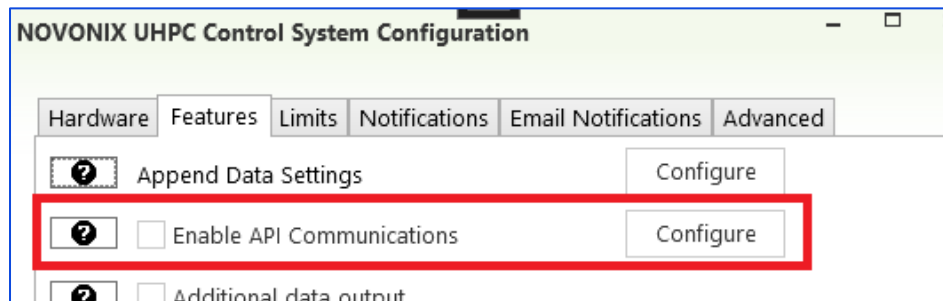



Figure 82: Enable API Communications

The API Communications Configuration page (Figure 83: Configure API Communications) is accessed by clicking the **Configure** button next to the "Enable API Communications" checkbox in the **Features** tab.

By default, the IP Address is set to 0.0.0.0. Allowing communications to the UHPC Control workstation from any connected network that permits traffic through port 11000. Alternatively, users can assign a specific IP for access over a particular network. In both cases, the user must know the workstations network IP. This can be obtained via the IT department, or by running "ipconfig" in the Windows command prompt.

The remaining options are a subset of the notification settings found in the **Notifications** tab of the UHPC Control System Configuration. When sending an API command, popups for actions like setting channel information or starting a test must be allowed or denied. If an action type is set to error, both the channel action and the API request response will result in failure.

Clicking any of the [?] icons next to a configuration option will display detailed information about that setting in the textbox at the bottom of the page.

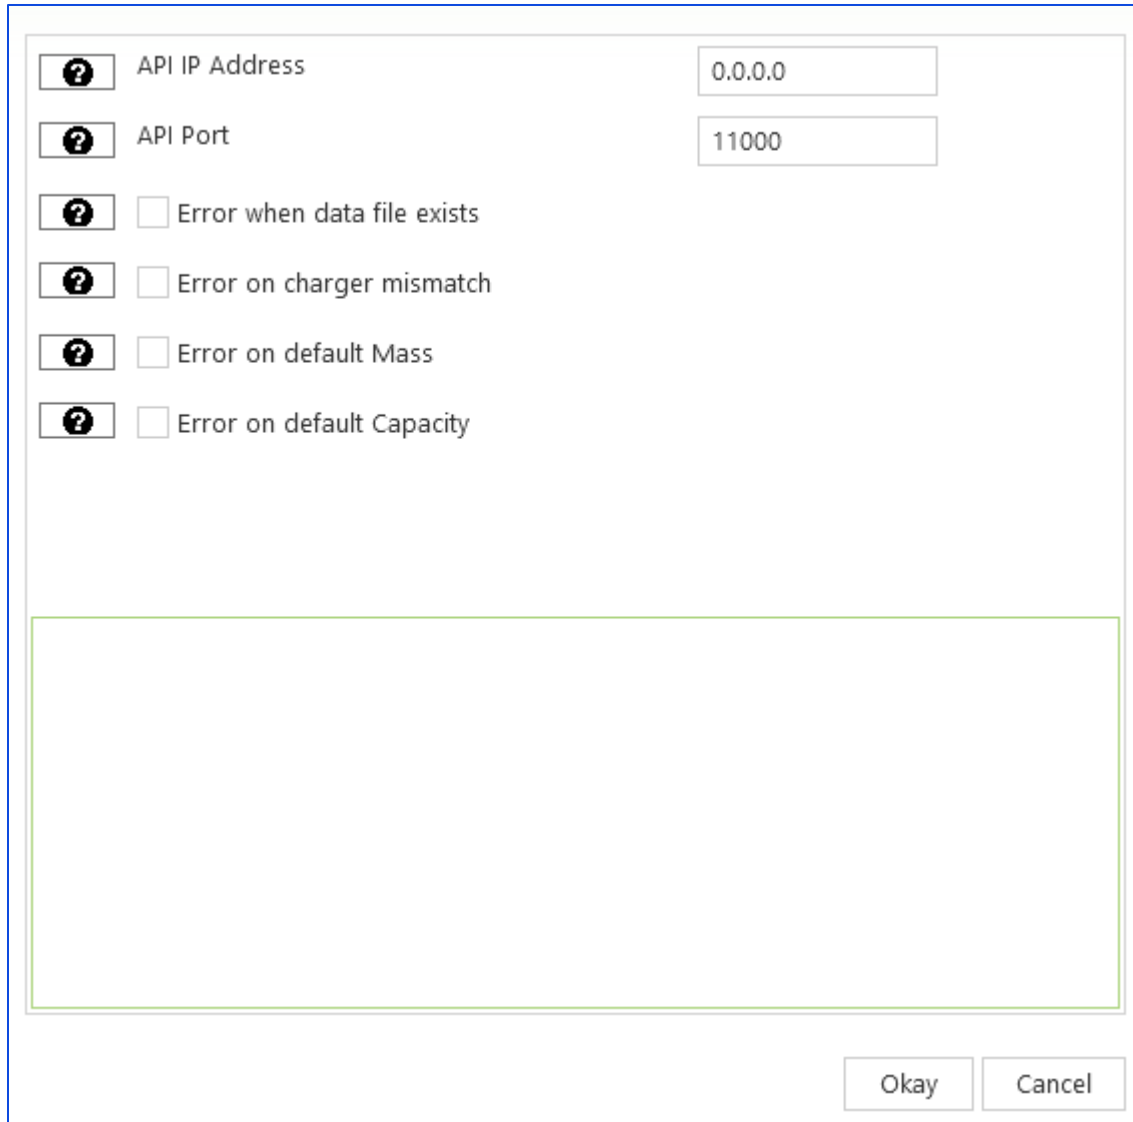

The dialog box titled "Configure API Communications" contains the following fields and options:

- API IP Address:** A text input field containing "0.0.0.0".
- API Port:** A text input field containing "11000".
- Error when data file exists:** An unchecked checkbox.
- Error on charger mismatch:** An unchecked checkbox.
- Error on default Mass:** An unchecked checkbox.
- Error on default Capacity:** An unchecked checkbox.

At the bottom right of the dialog are "Okay" and "Cancel" buttons. A large empty rectangular box is located below the checkbox options.

Figure 83: Configure API Communications

UHPC Control API Message Format

The API Message Format uses the JSON RPC 2.0 standard for all requests and responses. More detailed information can be found at <https://www.jsonrpc.org/specification>.

All requests to UHPC Control via the API will follow the format outlined in **Table 1: External UHPC Request**, with Parameters specified in **Table 2: UHPC Channel Request** or **Table 3: UHPC Channel Update Request**.

Responses from UHPC Control will confirm to the format described in **Table 4: External UHPC Success Response** or **Table 5: External UHPC Error Response**. The success response may contain a result with a list of objects defined in **Table 7: UHPC Channel Status**, while the error response may contain an error object outlined in **Table 6: JsonRequestError**.



The following sections will provide samples of each message type with descriptions of their functionality.

Name	Type	Description
jsonrpc	string	A String specifying the version of the JSON-RPC protocol. Must be exactly "2.0"
method	string	A String containing the name of the method to be invoked: getStatus, setChannelInfo, startChannel, stopChannel, suspendChannel, resumeChannel
id	String or int	An identifier established by the Client that must contain a String or Number. This isn't required to be unique between requests but helps differentiate the response.
params	UHPC Channel Request or UHPC Channel Update Request	JSON in the form of an object, containing the information server needs to handle request

Table 1: External UHPC Request

Name	Type	Description
channels	int[]	An integer array containing channel numbers. This array must not be empty, and must have valid channel number

Table 2: UHPC Channel Request

Name	Type	Description
channelNum (required)	int	Channel Number for request to update.
mass	string	Mass for channel.
capacity	string	Cell capacity for channel.
description	string	Description for the channel to be saved into the datafile and displayed in cell grid.
dataFilePath	string	Absolute path for datafile to be saved. Note: Must use / not \
protocolPath	string	Absolute path to find protocol file. Note: Must use / not \
ipAddress (optional)	string	Used to differentiate between master controllers when using Multi-System mode.
CellID	String	Sets the optional CellID display column and metadata

Table 3: UHPC Channel Update Request

Name	Type	Description
jsonrpc	string	A string specifying the version of the JSON-RPC protocol. Must be exactly "2.0".
result	string or UHPC Channel Status []	A string containing the word "SUCCESS" or an array of UHPC Channel Status objects.
id	string	The ID provided in the request.

Table 4: External UHPC Success Response

Name	Type	Description
jsonrpc	string	A String specifying the version of the JSON-RPC protocol. Must be exactly "2.0".
error	JsonRpcError	Object containing the error details.
id	string or int	An identifier established by the Client that must contain a string, or number.

Table 5: External UHPC Error Response

Name	Type	Description
code	int	Error codes: -32700: Parse error (Invalid JSON was received by the server, an error occurred on the server while parsing the JSON text). -32600: Invalid Request (JSON sent is not a valid Request object). -32601 Method not found (The method does not exist or is not available). -32602 Invalid params Invalid method parameter(s).
message	string	A string providing a short description of the error. The message should be limited to a concise single sentence.
data	string[]	A string array containing a detailed list of errors.

Table 6: JsonRpcError



Name	Type	Description
channelNumber	int	Channel Number.
status	string	Status of channel: Idle, Running, Completed, Suspended, Disabled, InError
mass	string	Mass set for channel.
cap	string	Cell capacity set for channel in AmpHours.
description	string	Description for the channel.
currentProtocolStepNumber	int	Current step number of protocol.
dataFilePath	string	Absolute path to the datafile.
protocolPath	string	Absolute path to the protocol file.
activeStepDisplay	string	String representing the current step being executed.
temp	string	Reported temperature of the cell.
runTime	string	Total run time of protocol in hours.
stepTime	string	Total run time of the active step in hours.
current	string	Current being applied to cell in Amps.
potential	string	Potential of cell in Volts.
cycleNum	string	Current cycle the protocol is on.

Table 7: UHPC Channel Status

Get Channel Status

The “Get Channel Status” format is an External UHPC Request that includes a list of channel numbers for parameters. It will return the channel information for the requested channels with a list of UHPC Channel Status objects described above.

Examples:

```
{
  "jsonrpc": "2.0",
  "method": "getStatus",
  "id": "1",
  "params": {
    "channels": [3]
  }
}
```

```
{
  "jsonrpc": "2.0",
  "method": "getStatus",
  "id": "ffa044c5-00de-4fce-90d7-ae5060a978f7",
  "params": {
    "channels": [1,10]
  }
}
```

Example Response:

```
{
  "jsonrpc": "2.0",
  "id": "ffa044c5-00de-4fce-90d7-ae5060a978f7",
  "result": [
    {
      "channelNumber": "01",
      "description": "API Description set",
      "status": "Running",
      "dataFilePath": "C:\\Users\\uhpc-dev.svc\\Desktop\\UHPC\\Protocols\\results\\2024-10-08_TC52_Run1_C1_CH01.csv",
      "protocolPath": "C:\\Users\\uhpc-dev.svc\\Desktop\\UHPC\\Protocols\\TC52_API.pro2",

```



```
"currentProtocolStepNumber": 1,
"activeStepDisplay": "Open Circuit Storage",
"temp": "22.208°C",
"runTime": "52.88 s",
"stepTime": "52.88 s",
"current": "0.00000000 A",
"potential": "1.57916114 V",
"cycleNum": "1/1",
"mass": "2.0",
"capacity": "2.0"
},
{
  "channelNumber": "10",
  "description": "Enter description here...",
  "status": "Idle",
  "dataFilePath": "",
  "protocolPath": "Click to select protocol file...",
  "currentProtocolStepNumber": 0,
  "activeStepDisplay": "---",
  "temp": "22.182°C",
  "runTime": "---",
  "stepTime": "---",
  "current": "---",
  "potential": "3.62160253 V",
  "cycleNum": "---",
  "mass": "1.000",
  "capacity": "1.000"
}
]
}}
```

Set Channel Info

The “Set Channel Info” format is an External UHPC Request that includes a list of UHPC Channel Update Requests for parameters. After setting the channel info, in the case of success, a simple UHPC Success Response will be returned.

Examples:

```
{"jsonrpc": "2.0",
  "method": "setChannelInfo",
  "id": "1b",
  "params": [{
    "channelNum": 1,
    "mass": "2.2",
    "capacity": "1.5",
    "description": "channel1description",
```



```
"dataFilePath": "C:/Avrion/TestResults/2024-09-21_TC01_R1.csv",  
"protocolPath": "C:/Avrion/ProtocolFiles/TC01_Delta_CC_ChargeConditionUnits.pro2"  
},  
{  
  "channelNum": 3,  
  "dataFilePath": "C:/Avrion/TestResults/2024-09-21_TC02_R1.csv",  
  "protocolPath": "C:/Avrion/ProtocolFiles/TC02_Delta_CC_DischargeConditionUnits.pro2",  
  "CellID": "#1541b"  
}}}
```

Start Channel

The “Start Channel” format is an External UHPC Request that includes a list of UHPC channel numbers for parameters. After starting the channels, in the case of success, a simple UHPC Success Response will be returned. If any channel fails to start, a UHPC Error Response will be returned.

Examples:

```
{"jsonrpc": "2.0", "method": "startChannel", "id": "54", "params": {"channels": [1]}}
```

```
{"jsonrpc": "2.0", "method": "startChannel", "id": "55", "params": {"channels": [1,2,3]}}
```

Stop Channel

The “Stop Channel” format is an External UHPC Request that includes a list of channel numbers for parameters. After stopping the channels, in the case of success, a simple UHPC Success Response will be returned. If any channel fails to stop, a UHPC Error Response will be returned.

Examples:

```
{"jsonrpc": "2.0", "method": "stopChannel", "id": "23", "params": {"channels": [2]}}
```

```
{"jsonrpc": "2.0", "method": "stopChannel", "id": "24", "params": {"channels": [1,2,3,4]}}
```

Suspend Channel

The “Suspend Channel” format is an External UHPC Request that includes a list of channel numbers for parameters. After suspending the channels, in the case of success, a simple UHPC Success Response will be returned. If any channel fails to suspend, a UHPC Error Response will be returned.



Examples:

```
{"jsonrpc": "2.0", "method": "suspendChannel", "id": "twelve", "params": {"channels": [8]}}
```

```
{"jsonrpc": "2.0", "method": "suspendChannel", "id": "thirteen", "params": {"channels": [1,2,3]}}
```

Resume Channel

The “Resume Channel” format is an External UHPC Request that includes a list of channel numbers for parameters. After resuming the channels, in the case of success, a simple UHPC Success Response will be returned. If any channel fails to resume, a UHPC Error Response will be returned.

Examples:

```
{"jsonrpc": "2.0", "method": "resumeChannel", "id": "1a", "params": {"channels": [3]}}
```

```
{"jsonrpc": "2.0", "method": "resumeChannel", "id": "1b", "params": {"channels": [2,3]}}
```

Clear Channel Info

The “Clear Channel Info” format is an External UHPC Request that includes a list of channel numbers for parameters. After clearing the channels, in the case of success, a simple UHPC Success Response will be returned. If any channel fails to clear, a UHPC Error Response will be returned.

Examples:

```
{"jsonrpc": "2.0", "method": "clearChannelInfo", "id": "1a", "params": {"channels": [3]}}
```

```
{"jsonrpc": "2.0", "method": "clearChannelInfo", "id": "1b", "params": {"channels": [2,3]}}
```

Sample Message Responses

The **SUCCESS** response for all message types is identical, as shown below. Note that **getStatus** is the exception, which is described in the [Get Channel Status](#) section above.

Additionally, below are a few sample error messages that may be returned:

Examples:

```
{  
  "jsonrpc": "2.0",
```



```
"result": "SUCCESS",
"id": "request_1"
}

{
  "jsonrpc": "2.0",
  "error": {
    "code": -32602,
    "message": "System: Sys1, Channel: 2: Channel 2: [Global Limit] Constant Current Charge Step 2
condition when voltage > 14.2 V ",
    "data": null
  },
  "id": "request_2"
}

{
  "jsonrpc": "2.0",
  "error": {
    "code": -32602,
    "message": "System: Sys1, Channel: 3, Cannot stop an idle channel.",
    "data": null
  },
  "id": "request_3"
}

{
  "jsonrpc": "2.0",
  "error": {
    "code": -32602,
    "message": "System: Sys1, Channel: 5, Cannot resume a idle channel.",
    "data": null
  },
  "id": "request_4"
}
```



Contact Us

Avrion Battery Labs
110 Simmonds Drive
Dartmouth, NS B3B 1N9
Support@Avrionlabs.com
+1 (782) 888-0528